


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021623\
Data File : VV030055.D
Acq On : 16 Feb 2023 09:28
Operator : SY/MD
Sample : BFB223
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB223

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM021523.M
Title : TRACE VOA SOM01.0
Last Update : Thu Feb 16 01:49:02 2023

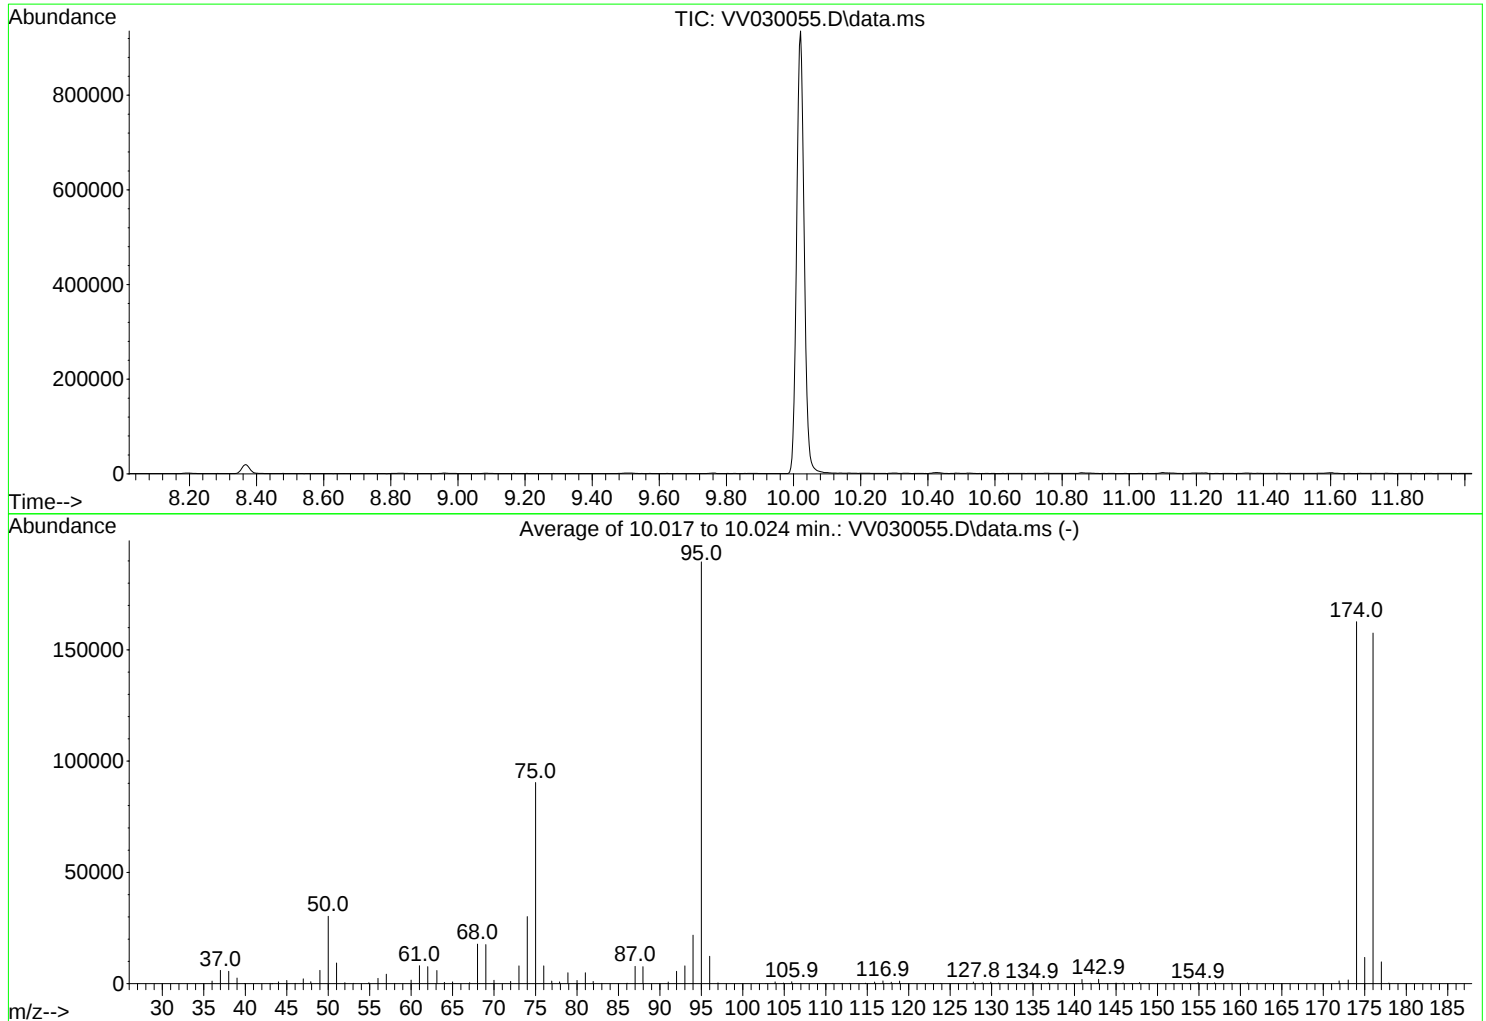

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2779

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	30253	PASS
75	95	30	80	47.7	90408	PASS
95	95	100	100	100.0	189568	PASS
96	95	5	9	6.5	12288	PASS
173	174	0.00	2	1.0	1654	PASS
174	95	50	120	85.8	162645	PASS
175	174	5	9	7.3	11803	PASS
176	174	95	101	96.9	157525	PASS
177	176	5	9	6.2	9807	PASS

m/z	Abundance
40.00	192.0
44.00	632.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

m/z	Abundance
36.00	1190.0
37.00	6097.0
38.00	5900.0
39.00	2636.0
39.90	242.0
43.00	108.0
43.20	108.0
44.00	1401.0
45.00	1448.0
46.00	205.0
47.00	2221.0
47.90	927.0
49.00	6100.0
50.00	31072.0
51.00	9761.0
52.00	410.0
53.10	132.0
54.90	393.0
56.00	2368.0
57.00	4602.0
58.00	156.0
60.00	1655.0
61.00	8088.0
62.00	8044.0
63.10	5957.0
64.00	581.0
65.00	862.0
67.00	415.0
68.00	18192.0
69.00	17752.0
70.00	1538.0
72.00	993.0
73.00	8007.0
74.00	30160.0
75.00	91080.0
76.00	8130.0
76.90	1218.0
77.90	774.0
78.90	5092.0
80.00	1466.0
81.00	4973.0
82.00	1042.0
83.00	130.0
86.10	226.0
87.00	8034.0
88.00	7543.0
91.00	762.0
92.00	5548.0
93.00	8150.0
94.00	21816.0
95.00	189888.0
96.00	12590.0
97.00	349.0
102.80	103.0
103.90	830.0
104.90	256.0
105.90	861.0
107.00	189.0
109.80	115.0
111.00	153.0
112.00	121.0
112.90	165.0
114.80	212.0
115.90	747.0
116.90	1227.0
117.90	666.0
118.90	1081.0
123.80	110.0
127.80	794.0
128.80	347.0
129.90	692.0
130.90	329.0
134.90	342.0
136.90	270.0
139.90	154.0
140.90	1870.0
141.90	214.0
142.90	2017.0
143.90	124.0
145.00	346.0
145.90	260.0
146.90	129.0
147.90	489.0
149.00	123.0
150.00	116.0
153.00	113.0
153.90	145.0
154.90	446.0
156.90	341.0
158.90	181.0
160.80	274.0
171.90	1314.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

173.00	1583.0
174.00	159744.0
175.00	11963.0
176.00	154432.0
177.00	9798.0
177.90	312.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

m/z	Abundance
36.00	1234.0
37.00	6121.0
38.00	5784.0
39.00	2588.0
39.90	252.0
43.00	157.0
44.00	1491.0
45.00	1481.0
46.00	166.0
47.00	2272.0
47.90	849.0
49.00	6146.0
50.00	31320.0
51.00	9565.0
52.00	419.0
53.00	121.0
54.90	461.0
56.00	2444.0
57.00	4401.0
58.00	154.0
60.00	1648.0
61.00	8341.0
62.00	7920.0
63.10	6032.0
64.00	623.0
65.00	831.0
67.10	418.0
68.00	18400.0
69.00	18088.0
70.00	1528.0
72.00	1066.0
73.00	8364.0
74.00	31200.0
75.00	93640.0
76.00	8282.0
76.90	1181.0
77.90	812.0
78.90	5066.0
80.00	1482.0
81.00	5054.0
81.90	1088.0
83.00	136.0
86.00	221.0
87.00	8072.0
87.90	7860.0
91.00	718.0
92.00	5740.0
93.00	8270.0
94.00	22544.0
95.00	195840.0
96.00	12772.0
97.00	365.0
102.80	121.0
103.90	826.0
104.90	280.0
105.90	870.0
107.00	174.0
109.80	103.0
110.80	154.0
111.90	139.0
112.90	170.0
114.80	229.0
115.90	708.0
116.90	1314.0
117.90	697.0
118.90	1181.0
123.80	150.0
127.80	755.0
128.80	330.0
129.90	715.0
130.90	298.0
134.90	385.0
136.90	301.0
139.90	161.0
140.90	1965.0
141.90	200.0
142.90	1997.0
145.00	303.0
145.90	273.0
146.90	141.0
147.80	524.0
149.00	119.0
150.00	161.0
151.90	104.0
152.80	131.0
153.80	155.0
154.90	501.0
156.90	359.0
159.00	203.0
160.90	302.0
171.90	1287.0
173.00	1683.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

174.00	168448.0
175.00	12219.0
176.00	163008.0
177.00	10124.0
177.90	294.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

m/z	Abundance
36.00	1143.0
37.00	5695.0
38.00	4976.0
39.00	2362.0
39.90	273.0
43.00	176.0
44.00	1437.0
45.00	1360.0
46.00	106.0
47.00	2062.0
47.90	777.0
49.00	5651.0
50.00	28368.0
51.00	8506.0
52.00	401.0
53.00	104.0
54.90	481.0
56.00	2336.0
57.00	3770.0
58.00	151.0
60.00	1515.0
61.00	7696.0
62.00	7019.0
63.10	5620.0
64.00	624.0
65.00	777.0
67.10	385.0
68.00	16600.0
69.00	16776.0
70.00	1390.0
72.00	984.0
73.00	7670.0
74.00	29040.0
75.00	86504.0
76.00	7596.0
77.00	1056.0
77.90	728.0
78.90	4569.0
80.00	1352.0
81.00	4654.0
81.90	984.0
83.00	137.0
86.00	206.0
87.00	7253.0
87.90	7386.0
91.00	646.0
92.00	5240.0
93.00	7553.0
94.00	20944.0
95.00	182976.0
96.00	11503.0
97.00	331.0
102.80	104.0
103.90	760.0
104.90	262.0
105.90	846.0
106.90	158.0
110.80	137.0
111.90	123.0
112.90	166.0
114.80	203.0
115.90	615.0
116.90	1208.0
117.90	672.0
118.90	1099.0
123.90	164.0
127.80	655.0
128.90	308.0
129.90	653.0
130.80	254.0
134.90	369.0
136.80	299.0
139.90	146.0
140.90	1877.0
141.90	190.0
142.90	1872.0
145.00	250.0
145.80	284.0
146.80	126.0
147.80	521.0
148.80	121.0
150.00	169.0
152.80	155.0
153.80	146.0
154.90	494.0
156.00	102.0
156.90	386.0
159.00	220.0
160.90	292.0
171.90	1177.0
173.00	1696.0
174.00	159744.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

175.00	11226.0
176.00	155136.0
177.00	9498.0
177.90	263.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223