
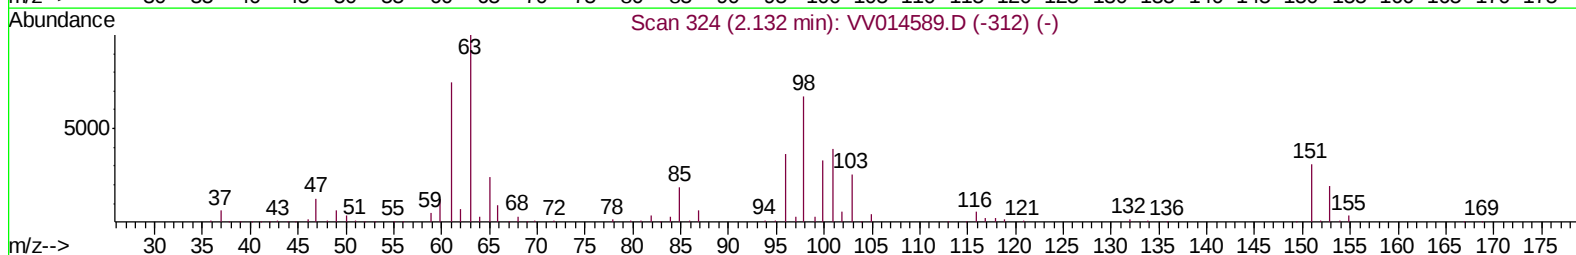
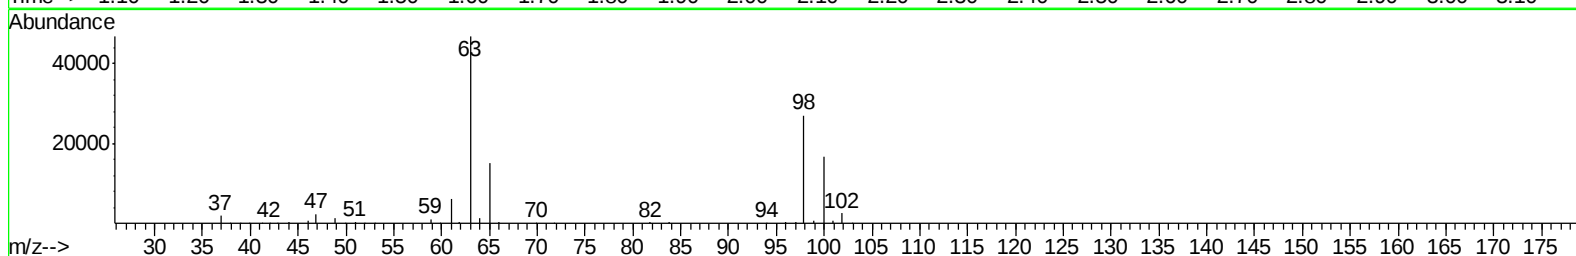


Data File : VV014593.D
Acq On : 17 Feb 2020 15:09
Operator : SY/MD
Sample : VV0217MBL05
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Feb 18 06:44:39 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM021720W.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 18 06:41:33 2020
Response via : Initial Calibration

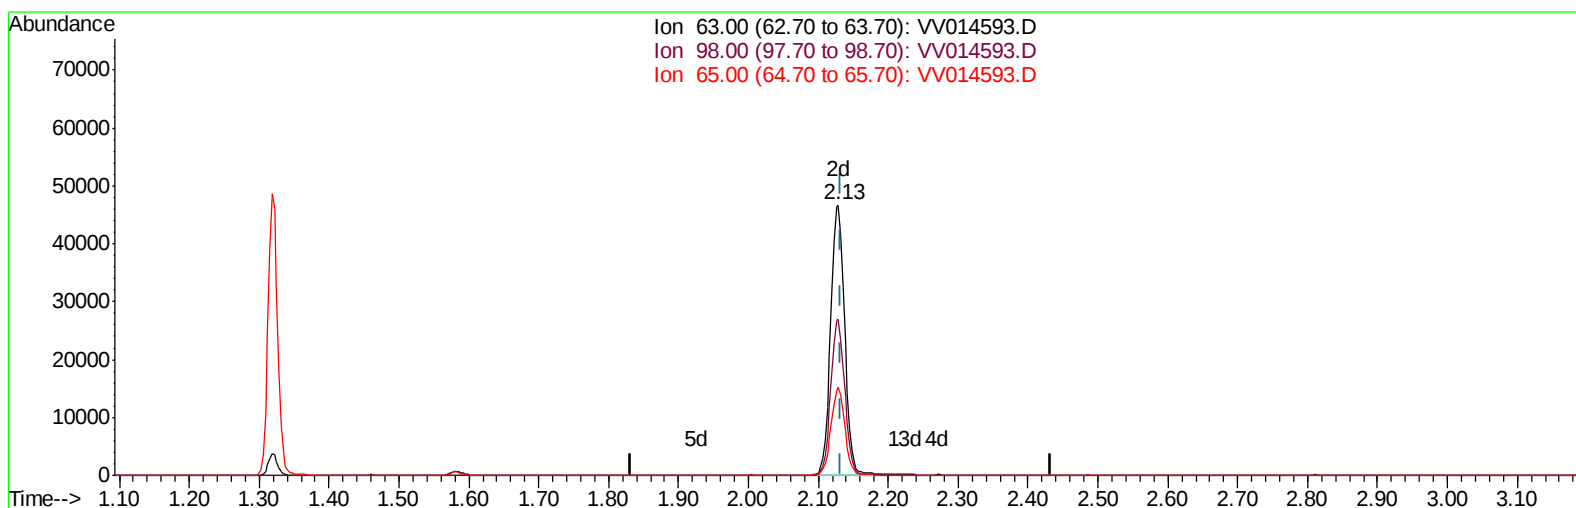

TIC: VV014593.D

(11) 1,1-Dichloroethene-d2 (S)

2.129min (-0.003) 36.11ug/L m

response 65317

Ion	Exp%	Act%
63.00	100	100
98.00	72.70	0.23#
65.00	22.70	0.10#
0.00	0.00	0.00