
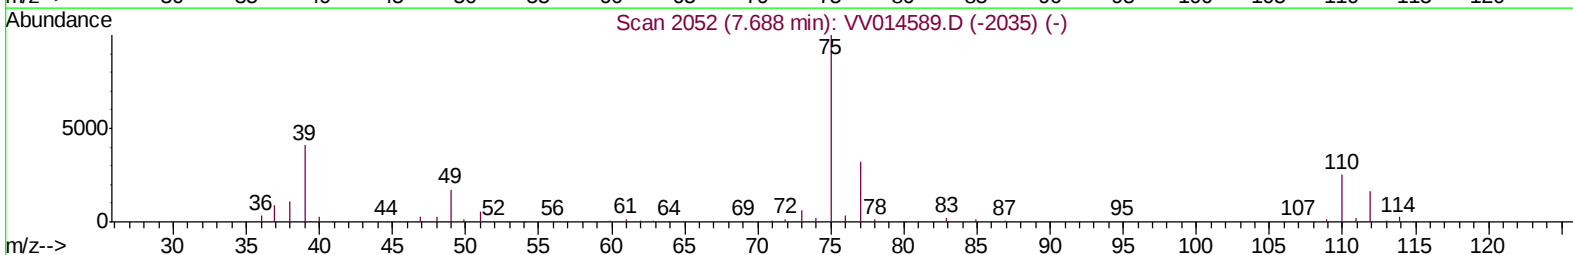
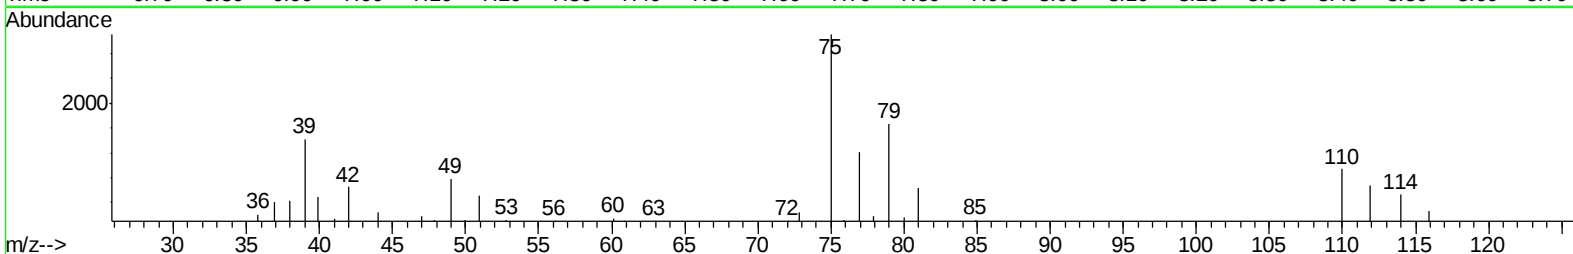


Data File : VV014596.D
Acq On : 17 Feb 2020 16:24
Operator : SY/MD
Sample : MDL05
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Feb 18 06:45:05 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM021720W.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 18 06:41:33 2020
Response via : Initial Calibration

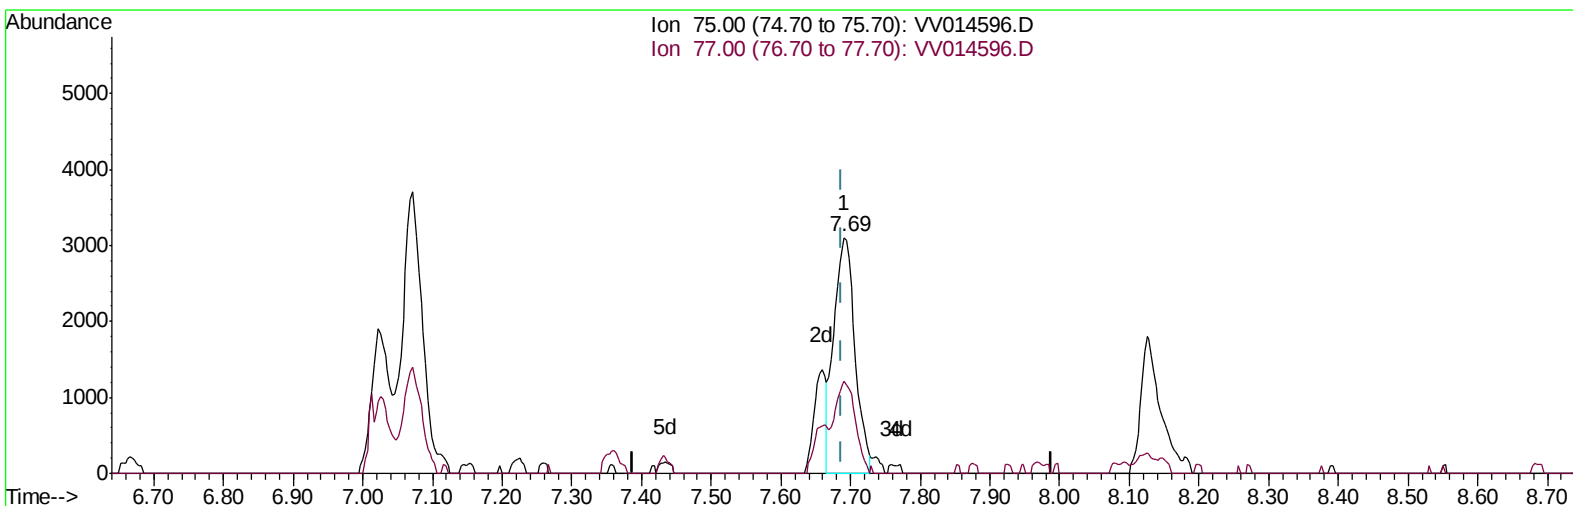

TIC: VV014596.D

(44) trans-1,3-Dichloropropene (T)

7.691min (+0.003) 2.28ug/L m

response 6496

Ion	Exp%	Act%
75.00	100	100
77.00	32.40	39.09
0.00	0.00	0.00
0.00	0.00	0.00