


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV021720\
 Data File : VV014586.D
 Acq On : 17 Feb 2020 10:35
 Operator : SY/MD
 Sample : BFB91
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB91

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM021720W.M
 Title : VOC Analysis
 Last Update : Tue Feb 18 06:41:33 2020

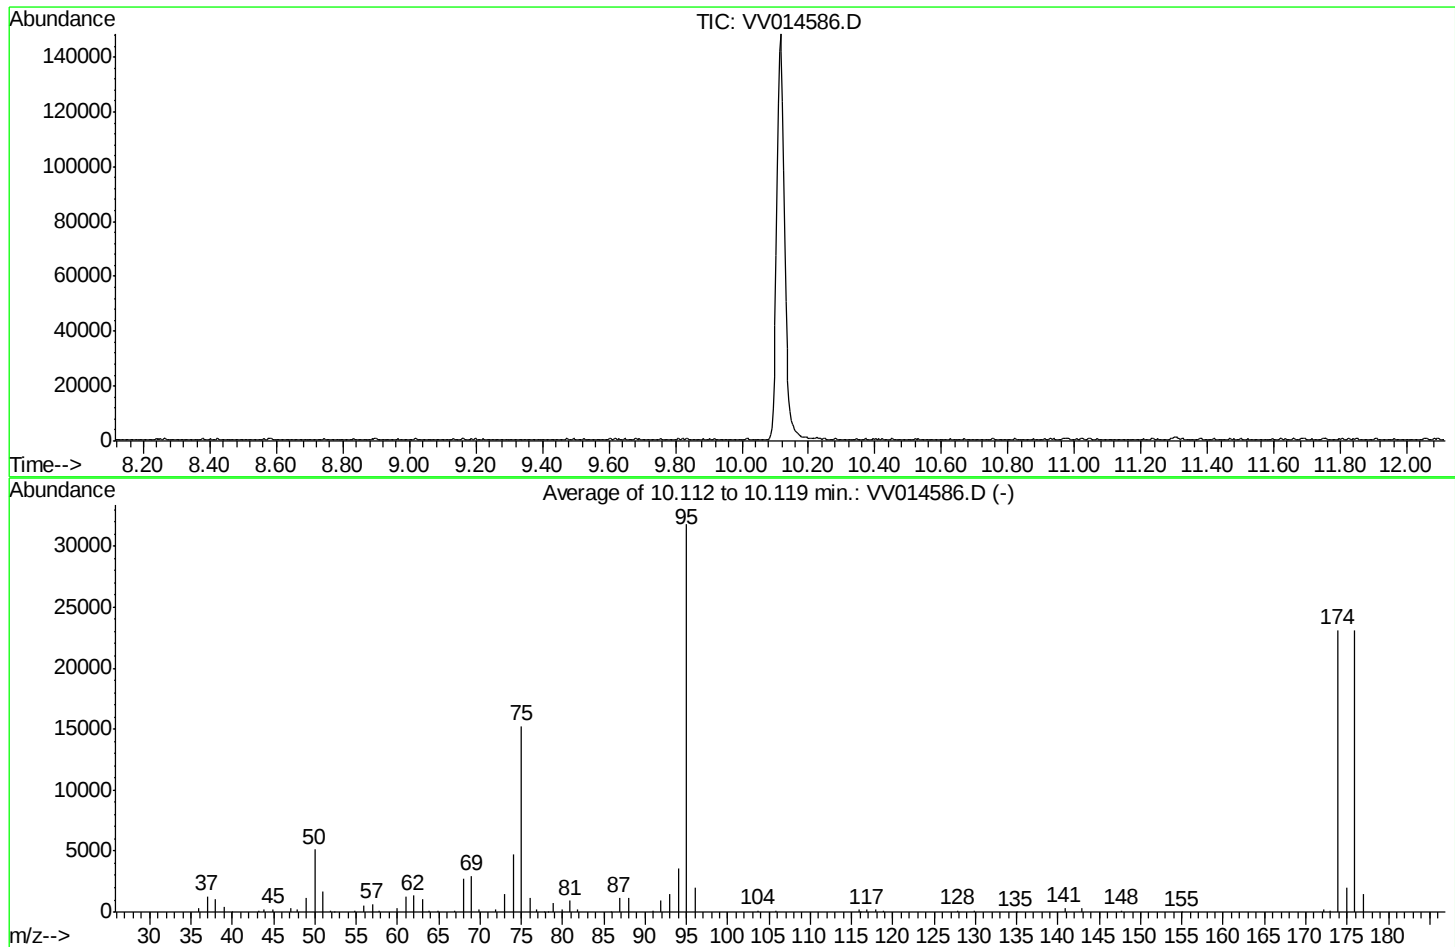

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	5140	PASS
75	95	30	80	47.9	15233	PASS
95	95	100	100	100.0	31797	PASS
96	95	5	9	6.4	2048	PASS
173	174	0.00	2	0.6	130	PASS
174	95	50	120	72.8	23144	PASS
175	174	5	9	8.7	2011	PASS
176	174	95	101	99.8	23101	PASS
177	176	5	9	6.4	1486	PASS

m/z	Abundance
35.90	268.0
37.00	1244.0
38.00	1123.0
39.00	450.0
39.90	219.0
43.90	493.0
45.00	277.0
47.10	317.0
47.90	265.0
49.00	1159.0
50.00	5090.0
51.00	1740.0
54.90	103.0
55.90	508.0
57.00	745.0
57.80	116.0
60.00	383.0
61.10	1301.0
62.00	1359.0
63.00	1024.0
66.90	109.0
68.00	2754.0
69.00	2932.0
69.90	250.0
72.00	190.0
73.00	1485.0
74.00	4748.0
75.00	14995.0
76.00	1266.0
76.90	223.0
77.80	124.0
78.80	725.0
80.00	236.0
80.90	931.0
81.80	212.0
86.80	1234.0
88.00	1050.0
91.90	867.0
92.90	1371.0
94.00	3540.0
95.00	31448.0
96.00	2165.0
103.70	164.0
105.80	127.0
115.80	147.0
116.10	141.0
116.80	230.0
118.00	181.0
118.80	170.0
127.80	169.0
129.90	138.0
140.80	301.0
142.80	349.0
147.70	111.0
172.10	140.0
172.90	392.0
173.90	22400.0
175.00	1857.0
175.90	22496.0
176.90	1409.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
35.90	296.0
37.00	1344.0
38.00	1088.0
39.00	443.0
39.90	244.0
43.20	120.0
43.90	457.0
44.90	277.0
47.00	366.0
47.90	238.0
49.00	1184.0
50.00	5297.0
51.00	1763.0
51.90	118.0
52.30	107.0
54.80	119.0
56.00	512.0
57.00	687.0
57.80	111.0
59.90	335.0
61.10	1299.0
62.00	1394.0
63.00	1038.0
63.90	111.0
64.90	107.0
66.90	109.0
68.00	2801.0
69.00	3029.0
69.90	269.0
71.90	175.0
73.00	1521.0
74.00	4939.0
75.00	15668.0
76.00	1230.0
76.90	260.0
78.90	748.0
79.90	265.0
80.90	943.0
81.80	234.0
86.80	1258.0
88.00	1143.0
91.00	113.0
92.00	943.0
92.90	1517.0
94.00	3703.0
95.00	32888.0
96.00	2087.0
103.70	151.0
105.80	136.0
115.80	187.0
116.90	190.0
117.90	172.0
118.90	157.0
127.80	151.0
129.90	147.0
140.80	358.0
142.80	361.0
147.70	137.0
172.10	188.0
173.90	23816.0
175.00	2070.0
175.90	23792.0
176.90	1519.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
35.90	266.0
37.00	1312.0
38.00	921.0
38.90	410.0
39.90	259.0
43.10	134.0
43.90	416.0
44.90	241.0
47.00	374.0
47.90	199.0
49.00	1168.0
50.00	5035.0
51.00	1539.0
51.90	137.0
54.80	104.0
56.00	415.0
56.90	619.0
59.80	298.0
61.10	1253.0
61.90	1287.0
63.00	1035.0
63.80	144.0
64.90	114.0
68.00	2628.0
68.90	2935.0
69.90	258.0
71.90	162.0
73.00	1366.0
74.00	4635.0
75.00	15037.0
76.00	1069.0
76.90	280.0
78.20	153.0
78.90	692.0
79.90	271.0
80.90	902.0
81.80	222.0
85.90	105.0
86.90	1108.0
87.90	1213.0
90.90	154.0
92.00	883.0
93.00	1448.0
94.00	3563.0
95.00	31056.0
96.10	1892.0
103.70	144.0
105.80	126.0
115.90	197.0
117.00	167.0
117.90	147.0
119.00	151.0
127.90	144.0
129.90	156.0
134.90	105.0
140.80	384.0
142.80	327.0
147.70	145.0
155.00	114.0
172.10	197.0
173.90	23216.0
174.90	2106.0
175.90	23016.0
176.90	1531.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

Scan 2795 (10.077 min): VV014586.D
BFB91

m/z	Abundance
35.60	102.0
40.10	185.0
43.90	229.0
45.80	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91