

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021721\
 Data File : VV020339.D
 Acq On : 17 Feb 2021 11:05
 Operator : SY/MD
 Sample : VV0217WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	355569	353457	15.56%	2.049%
2	1.568	156	164	181	rBV	291312	327448	14.41%	1.898%
3	2.108	321	332	361	rVB	578297	884534	38.94%	5.127%
4	2.256	374	378	381	rBV3	420	308	0.01%	0.002%
5	2.288	386	388	389	rBV	613	241	0.01%	0.001%
6	2.362	408	411	414	rVV3	480	313	0.01%	0.002%
7	2.513	451	458	466	rVB5	2085	3417	0.15%	0.020%
8	2.542	466	467	472	rBV2	309	227	0.01%	0.001%
9	2.606	483	487	489	rBV3	439	248	0.01%	0.001%
10	2.709	515	519	522	rBV2	219	217	0.01%	0.001%
11	2.764	532	536	538	rBV4	367	295	0.01%	0.002%
12	2.815	549	552	556	rVV	485	270	0.01%	0.002%
13	2.834	556	558	563	rVB4	311	222	0.01%	0.001%
14	2.899	575	578	581	rBV2	311	231	0.01%	0.001%
15	3.076	629	633	635	rVV2	340	272	0.01%	0.002%
16	3.310	702	706	712	rVB	281	279	0.01%	0.002%
17	3.397	726	733	736	rBV	440	305	0.01%	0.002%
18	3.510	765	768	772	rVV2	220	230	0.01%	0.001%
19	3.539	773	777	781	rVV2	358	323	0.01%	0.002%
20	3.577	787	789	794	rBV3	296	218	0.01%	0.001%
21	3.883	874	884	922	rBV	144545	422603	18.60%	2.449%
22	4.352	1013	1030	1060	rBV	362802	908183	39.98%	5.264%
23	4.539	1086	1088	1090	rBV2	548	328	0.01%	0.002%
24	4.722	1142	1145	1150	rVB2	484	343	0.02%	0.002%
25	4.805	1166	1171	1173	rBV3	397	343	0.02%	0.002%
26	4.928	1203	1209	1210	rBV2	219	238	0.01%	0.001%
27	5.050	1228	1247	1280	rBV2	884360	2271682	100.00%	13.167%
28	5.362	1341	1344	1347	rVB3	579	304	0.01%	0.002%
29	5.384	1347	1351	1353	rBV2	482	351	0.02%	0.002%
30	5.474	1374	1379	1380	rBV2	489	338	0.01%	0.002%
31	5.619	1410	1424	1455	rBV	644037	1305205	57.46%	7.565%
32	5.799	1477	1480	1482	rBV2	589	306	0.01%	0.002%
33	5.860	1497	1499	1502	rVB2	490	269	0.01%	0.002%
34	5.911	1502	1515	1530	rBV2	28043	59493	2.62%	0.345%
35	6.072	1550	1565	1593	rBV	495291	1011109	44.51%	5.861%
36	6.265	1621	1625	1631	rVB4	640	719	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021721\
 Data File : VV020339.D
 Acq On : 17 Feb 2021 11:05
 Operator : SY/MD
 Sample : VV0217WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

37	6.304	1635	1637	1641	rVB4	393	273	0.01%	0.002%
38	6.323	1641	1643	1648	rVB3	461	314	0.01%	0.002%
39	6.352	1648	1652	1655	rBV	522	468	0.02%	0.003%
40	6.490	1689	1695	1698	rVB	265	231	0.01%	0.001%
41	6.510	1698	1701	1705	rBV	416	302	0.01%	0.002%
42	6.638	1738	1741	1743	rBV3	503	329	0.01%	0.002%
43	6.699	1758	1760	1766	rVB3	353	266	0.01%	0.002%
44	6.921	1825	1829	1832	rBV2	322	255	0.01%	0.001%
45	6.989	1837	1850	1881	rBV	262835	484321	21.32%	2.807%
46	7.255	1931	1933	1939	rVB4	757	536	0.02%	0.003%
47	7.320	1939	1953	1979	rBV	1069301	1831245	80.61%	10.614%
48	7.625	2037	2048	2076	rBV	186019	325262	14.32%	1.885%
49	7.802	2099	2103	2106	rBV3	485	318	0.01%	0.002%
50	7.934	2142	2144	2150	rVB4	434	391	0.02%	0.002%
51	7.963	2150	2153	2156	rBV2	293	249	0.01%	0.001%
52	7.992	2160	2162	2168	rVB2	810	492	0.02%	0.003%
53	8.091	2182	2193	2227	rBV2	501387	955859	42.08%	5.540%
54	8.419	2290	2295	2296	rBV4	856	702	0.03%	0.004%
55	8.497	2315	2319	2321	rBV3	573	387	0.02%	0.002%
56	8.538	2330	2332	2335	rBV3	496	284	0.01%	0.002%
57	8.657	2368	2369	2375	rVB2	524	368	0.02%	0.002%
58	8.747	2394	2397	2402	rVB3	355	310	0.01%	0.002%
59	8.776	2402	2406	2407	rBV2	577	291	0.01%	0.002%
60	8.857	2418	2431	2462	rBV	1004548	1630326	71.77%	9.450%
61	9.034	2481	2486	2491	rVB5	530	591	0.03%	0.003%
62	9.082	2499	2501	2505	rVB2	612	353	0.02%	0.002%
63	9.140	2513	2519	2521	rBV4	423	467	0.02%	0.003%
64	9.548	2642	2646	2647	rVV2	348	234	0.01%	0.001%
65	9.683	2684	2688	2692	rBV2	304	331	0.01%	0.002%
66	9.834	2732	2735	2739	rVB	490	329	0.01%	0.002%
67	9.886	2748	2751	2756	rBV2	244	214	0.01%	0.001%
68	10.088	2810	2814	2816	rBV3	261	222	0.01%	0.001%
69	10.223	2843	2856	2881	rBV	671499	1046433	46.06%	6.065%
70	10.390	2902	2908	2914	rBV4	563	663	0.03%	0.004%
71	10.789	3028	3032	3037	rVB2	399	417	0.02%	0.002%
72	11.120	3131	3135	3138	rBV2	256	222	0.01%	0.001%
73	11.175	3147	3152	3153	rVV2	669	507	0.02%	0.003%
74	11.194	3155	3158	3164	rVB5	988	1015	0.04%	0.006%
75	11.255	3164	3177	3200	rBV	1084860	1630680	71.78%	9.452%
76	11.525	3259	3261	3266	rVB3	459	259	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021721\
 Data File : VV020339.D
 Acq On : 17 Feb 2021 11:05
 Operator : SY/MD
 Sample : VV0217WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	11.632	3281	3294	3316	rBV	1157940	1768327	77.84%	10.249%
78	12.024	3413	3416	3418	rBV2	400	224	0.01%	0.001%
79	12.053	3423	3425	3431	rVB3	330	324	0.01%	0.002%
80	12.265	3484	3491	3496	rBV5	942	1196	0.05%	0.007%
81	12.355	3516	3519	3521	rBV	309	235	0.01%	0.001%
82	12.377	3524	3526	3531	rVV3	252	232	0.01%	0.001%
83	12.448	3546	3548	3551	rVB2	380	223	0.01%	0.001%
84	12.487	3555	3560	3561	rBV2	302	270	0.01%	0.002%
85	12.529	3571	3573	3577	rVB2	435	249	0.01%	0.001%
86	12.664	3609	3615	3623	rVB6	845	1227	0.05%	0.007%
87	13.024	3724	3727	3730	rBV3	319	223	0.01%	0.001%
88	13.172	3770	3773	3774	rBV	400	235	0.01%	0.001%
89	13.275	3801	3805	3813	rBV5	1047	1239	0.05%	0.007%
90	13.339	3822	3825	3828	rBV2	458	401	0.02%	0.002%
91	13.394	3839	3842	3846	rBV3	417	317	0.01%	0.002%
92	13.525	3880	3883	3886	rBV	847	633	0.03%	0.004%
93	13.570	3894	3897	3901	rBV2	562	375	0.02%	0.002%
94	13.721	3942	3944	3947	rBV	447	234	0.01%	0.001%
95	14.664	4235	4237	4240	rBV3	388	290	0.01%	0.002%
96	14.847	4291	4294	4299	rBV3	746	705	0.03%	0.004%
97	14.950	4324	4326	4331	rBV2	489	329	0.01%	0.002%
98	15.316	4436	4440	4443	rBV6	872	843	0.04%	0.005%
99	15.368	4454	4456	4458	rBV2	839	503	0.02%	0.003%
100	15.509	4495	4500	4501	rBV4	3344	2506	0.11%	0.015%




Sum of corrected areas: 17252925

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021721\
Data File : VV020339.D
Acq On : 17 Feb 2021 11:05
Operator : SY/MD
Sample : VV0217WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

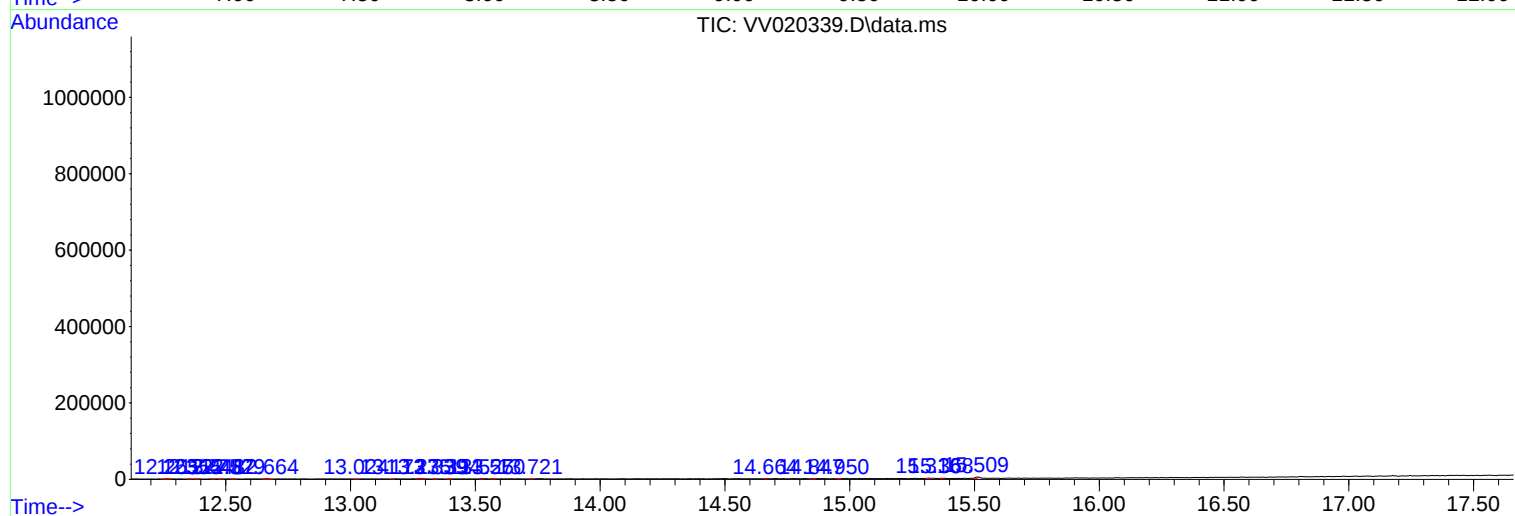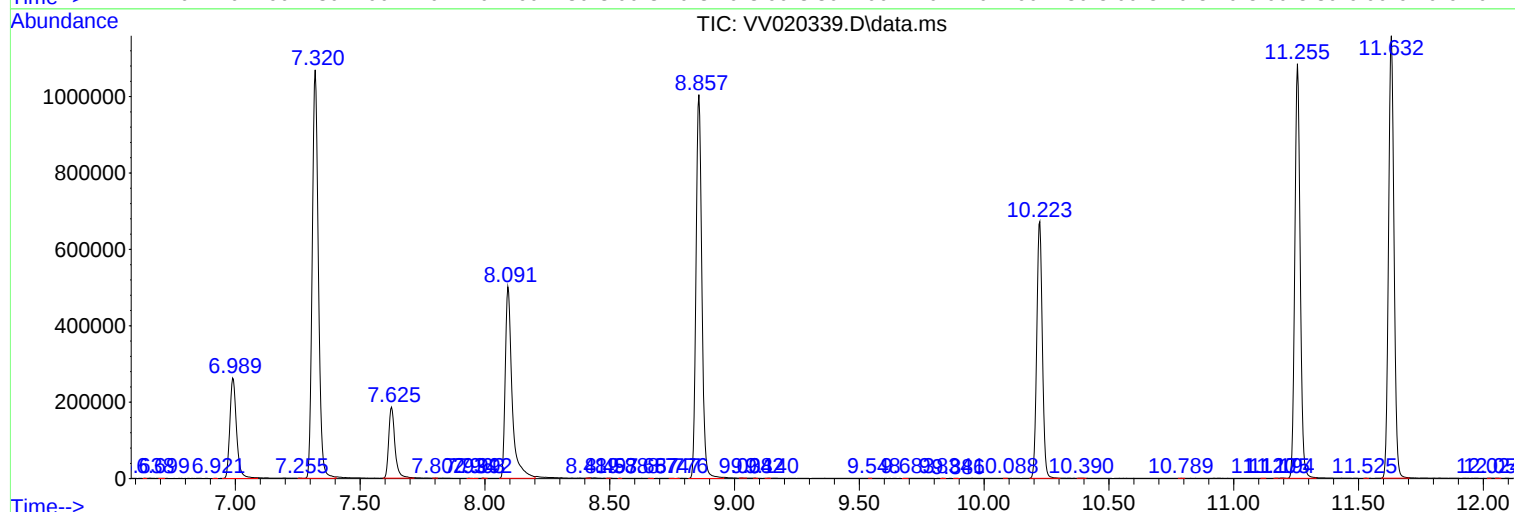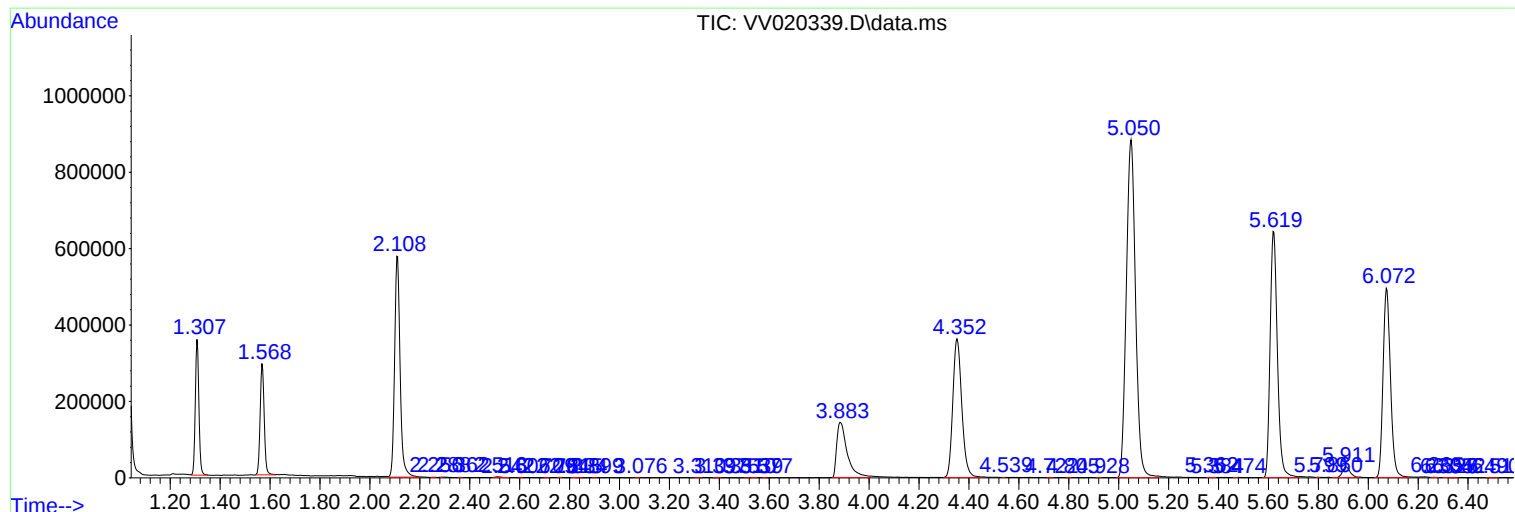

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021721\
Data File : VV020339.D
Acq On : 17 Feb 2021 11:05
Operator : SY/MD
Sample : VV0217WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021721\
Data File : VV020339.D
Acq On : 17 Feb 2021 11:05
Operator : SY/MD
Sample : VV0217WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
