

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021721\
 Data File : VW020341.D
 Acq On : 17 Feb 2021 12:44
 Operator : SY/MD
 Sample : VIBLK63
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VW020341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rVB	299218	301866	14.40%	1.915%
2	1.564	156	163	178	rVB	264474	298523	14.24%	1.894%
3	2.108	321	332	360	rVB	496107	750000	35.77%	4.759%
4	2.236	371	372	375	rBV2	417	238	0.01%	0.002%
5	2.281	384	386	397	rVB2	652	583	0.03%	0.004%
6	2.333	397	402	404	rBV2	297	305	0.01%	0.002%
7	2.510	448	457	463	rBV4	2063	2975	0.14%	0.019%
8	2.648	496	500	504	rBV2	311	232	0.01%	0.001%
9	2.670	504	507	512	rVB	356	298	0.01%	0.002%
10	2.760	531	535	541	rVV2	311	378	0.02%	0.002%
11	3.223	671	679	683	rBV2	298	361	0.02%	0.002%
12	3.246	683	686	690	rBV2	284	242	0.01%	0.002%
13	3.371	719	725	727	rBV3	252	209	0.01%	0.001%
14	3.606	795	798	801	rVB2	412	226	0.01%	0.001%
15	3.638	801	808	812	rBV	462	425	0.02%	0.003%
16	3.841	867	871	873	rBV2	312	199	0.01%	0.001%
17	3.879	873	883	920	rBV	145337	405781	19.35%	2.575%
18	4.272	1002	1005	1008	rBV2	342	290	0.01%	0.002%
19	4.352	1012	1030	1066	rBV	335372	839140	40.02%	5.324%
20	4.503	1075	1077	1083	rVB3	493	288	0.01%	0.002%
21	4.957	1216	1218	1224	rVB2	395	230	0.01%	0.001%
22	5.050	1228	1247	1274	rBV2	807830	2096954	100.00%	13.304%
23	5.207	1294	1296	1303	rVB5	1143	1081	0.05%	0.007%
24	5.252	1306	1310	1318	rVB5	1142	1359	0.06%	0.009%
25	5.291	1319	1322	1324	rBV3	832	450	0.02%	0.003%
26	5.313	1325	1329	1331	rBV3	380	227	0.01%	0.001%
27	5.619	1411	1424	1454	rBV	595405	1186374	56.58%	7.527%
28	5.834	1489	1491	1496	rBV2	398	306	0.01%	0.002%
29	5.911	1501	1515	1537	rVV2	31513	66010	3.15%	0.419%
30	5.992	1538	1540	1545	rVB2	276	202	0.01%	0.001%
31	6.072	1550	1565	1594	rBV	472033	952193	45.41%	6.041%
32	6.256	1620	1622	1625	rVV3	396	212	0.01%	0.001%
33	6.284	1629	1631	1633	rVB	519	230	0.01%	0.001%
34	6.304	1633	1637	1640	rVB3	477	468	0.02%	0.003%
35	6.326	1640	1644	1647	rBV3	277	212	0.01%	0.001%
36	6.542	1704	1711	1713	rBV2	245	211	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021721\
 Data File : VW020341.D
 Acq On : 17 Feb 2021 12:44
 Operator : SY/MD
 Sample : VIBLK63
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	6.577	1718	1722	1725	rBV2	264	221	0.01%	0.001%
38	6.648	1740	1744	1745	rVV2	298	233	0.01%	0.001%
39	6.657	1745	1747	1753	rVB4	509	356	0.02%	0.002%
40	6.902	1817	1823	1825	rBV	247	249	0.01%	0.002%

41	6.989	1837	1850	1875	rBV	241047	437182	20.85%	2.774%
42	7.169	1902	1906	1907	rBV2	456	306	0.01%	0.002%
43	7.243	1925	1929	1932	rVB3	445	351	0.02%	0.002%
44	7.320	1940	1953	1984	rBV	953905	1638891	78.16%	10.398%
45	7.625	2037	2048	2070	rBV2	170952	294981	14.07%	1.872%

46	7.982	2154	2159	2160	rBV3	390	355	0.02%	0.002%
47	8.091	2182	2193	2236	rBV2	464718	911001	43.44%	5.780%
48	8.294	2254	2256	2259	rVB3	874	468	0.02%	0.003%
49	8.381	2281	2283	2286	rVB2	990	417	0.02%	0.003%
50	8.400	2286	2289	2290	rBV2	370	233	0.01%	0.001%

51	8.416	2291	2294	2296	rBV2	880	644	0.03%	0.004%
52	8.487	2313	2316	2320	rBV3	519	381	0.02%	0.002%
53	8.558	2335	2338	2342	rVB3	551	305	0.01%	0.002%
54	8.603	2347	2352	2353	rBV2	435	309	0.01%	0.002%
55	8.619	2353	2357	2361	rBV4	556	367	0.02%	0.002%

56	8.722	2385	2389	2393	rVB2	506	447	0.02%	0.003%
57	8.792	2408	2411	2413	rBV2	374	242	0.01%	0.002%
58	8.857	2419	2431	2453	rBV	930343	1491504	71.13%	9.463%
59	9.117	2507	2512	2517	rBV2	628	390	0.02%	0.002%
60	9.313	2567	2573	2575	rBV2	292	271	0.01%	0.002%

61	9.329	2575	2578	2584	rVB	354	290	0.01%	0.002%
62	9.712	2694	2697	2702	rVB2	291	245	0.01%	0.002%
63	9.863	2741	2744	2750	rBV2	203	215	0.01%	0.001%
64	10.130	2824	2827	2834	rVB2	423	366	0.02%	0.002%
65	10.175	2834	2841	2843	rBV2	405	394	0.02%	0.002%

66	10.223	2843	2856	2881	rVV	625300	979476	46.71%	6.214%
67	10.413	2913	2915	2919	rVB2	394	216	0.01%	0.001%
68	10.532	2946	2952	2954	rBV2	266	308	0.01%	0.002%
69	10.548	2954	2957	2966	rVB4	466	570	0.03%	0.004%
70	10.741	3014	3017	3021	rBV2	382	329	0.02%	0.002%

71	10.857	3051	3053	3060	rVB2	544	423	0.02%	0.003%
72	10.895	3060	3065	3069	rBV	328	291	0.01%	0.002%
73	10.976	3085	3090	3092	rBV	395	445	0.02%	0.003%
74	10.992	3092	3095	3100	rVV2	495	462	0.02%	0.003%
75	11.024	3101	3105	3111	rVV3	325	349	0.02%	0.002%

76	11.181	3151	3154	3157	rBV	437	347	0.02%	0.002%
----	--------	------	------	------	-----	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021721\
 Data File : VV020341.D
 Acq On : 17 Feb 2021 12:44
 Operator : SY/MD
 Sample : VIBLK63
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	11.255	3166	3177	3200	rBV	960640	1460531	69.65%	9.267%
78	11.583	3274	3279	3281	rBV2	456	352	0.02%	0.002%
79	11.632	3281	3294	3316	rBV	1031796	1601435	76.37%	10.161%
80	11.863	3361	3366	3367	rBV3	518	340	0.02%	0.002%
81	11.898	3373	3377	3380	rVB3	373	312	0.01%	0.002%
82	11.914	3380	3382	3387	rBV	348	268	0.01%	0.002%
83	12.075	3427	3432	3434	rBV3	454	361	0.02%	0.002%
84	12.133	3447	3450	3452	rBV3	490	290	0.01%	0.002%
85	12.255	3482	3488	3491	rBV3	902	939	0.04%	0.006%
86	12.361	3518	3521	3524	rVB	387	217	0.01%	0.001%
87	12.439	3542	3545	3549	rVB2	334	201	0.01%	0.001%
88	12.603	3591	3596	3599	rBV2	426	354	0.02%	0.002%
89	12.667	3610	3616	3621	rVB4	461	521	0.02%	0.003%
90	12.895	3685	3687	3690	rBV	319	261	0.01%	0.002%
91	13.011	3721	3723	3726	rBV	322	252	0.01%	0.002%
92	13.609	3907	3909	3914	rBV2	414	335	0.02%	0.002%
93	13.709	3937	3940	3941	rBV	425	218	0.01%	0.001%
94	13.811	3970	3972	3975	rBV2	392	270	0.01%	0.002%
95	13.927	4004	4008	4011	rBV3	313	316	0.02%	0.002%
96	14.046	4042	4045	4046	rBV	513	243	0.01%	0.002%
97	14.818	4283	4285	4287	rVB	701	241	0.01%	0.002%
98	15.146	4383	4387	4393	rVB5	2022	2185	0.10%	0.014%
99	15.323	4435	4442	4450	rVB7	3830	5259	0.25%	0.033%
100	15.512	4494	4501	4510	rVB6	8440	11441	0.55%	0.073%




Sum of corrected areas: 15761250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021721\
Data File : VV020341.D
Acq On : 17 Feb 2021 12:44
Operator : SY/MD
Sample : VIBLK63
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

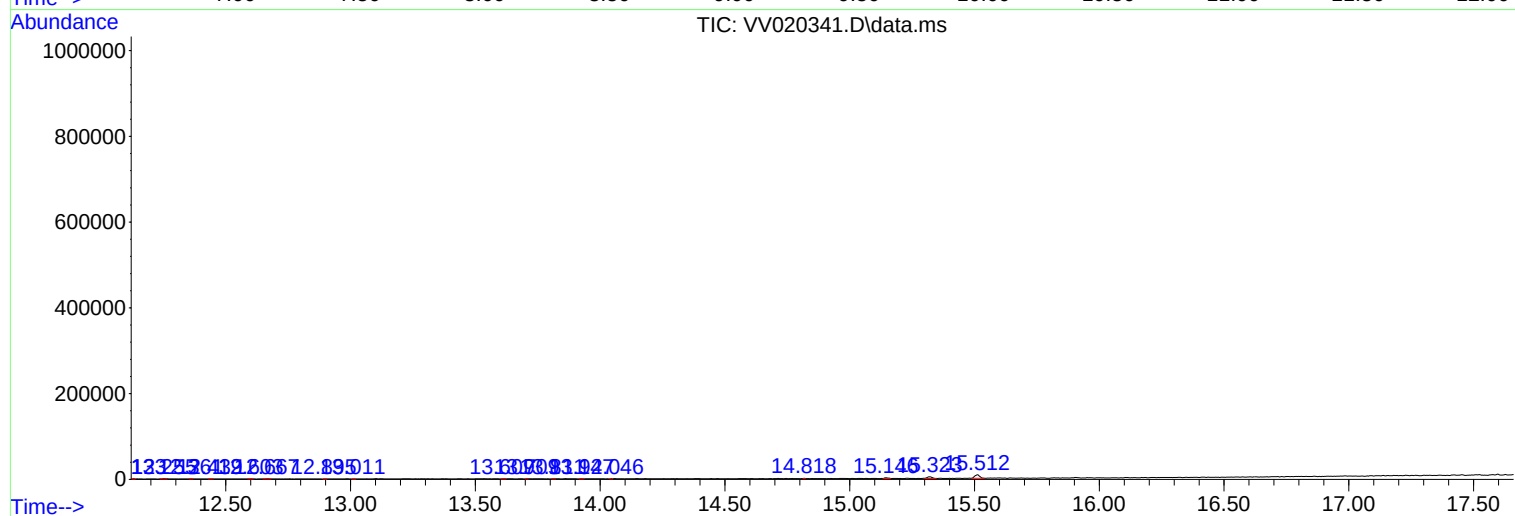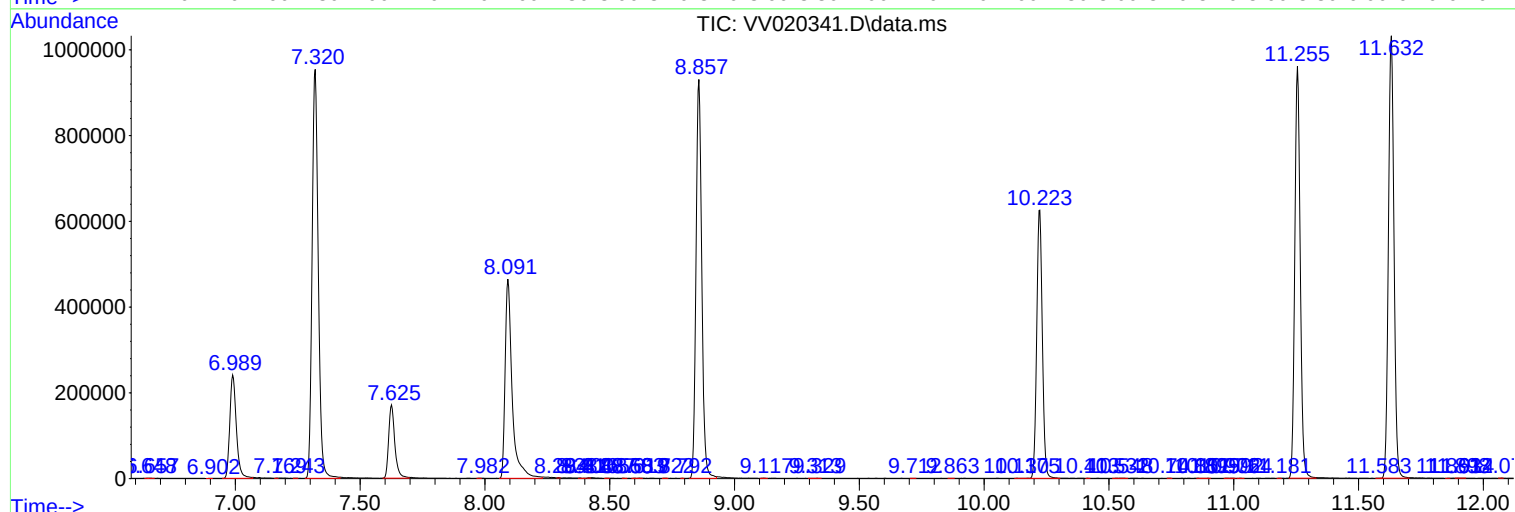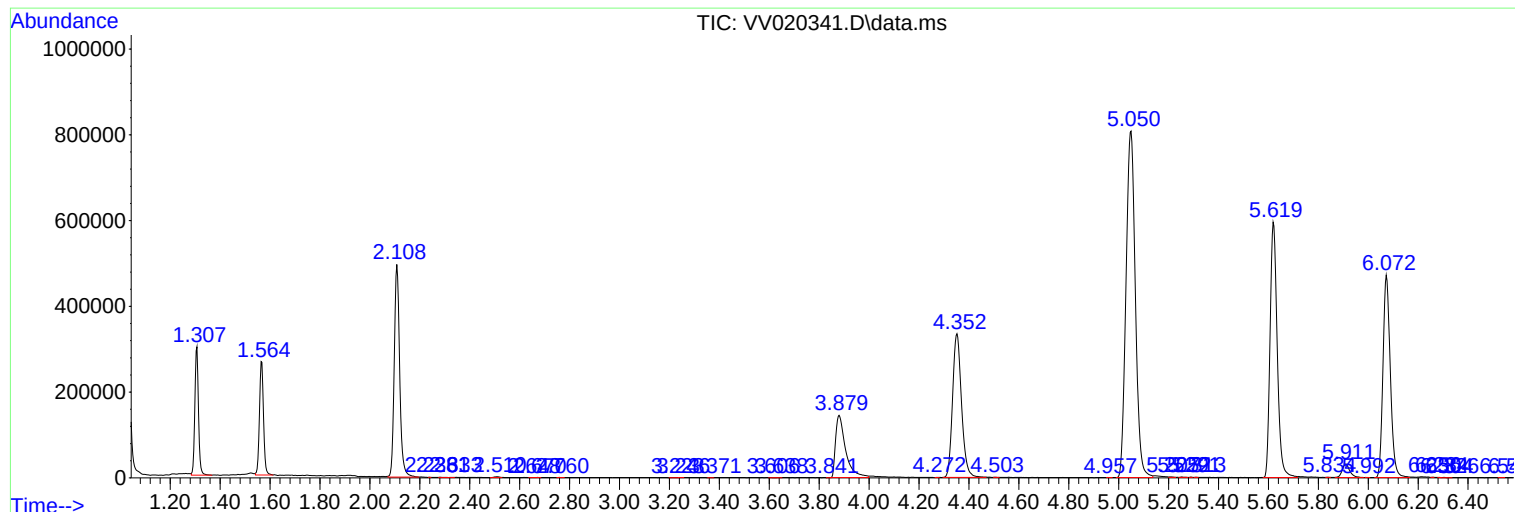

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021721\
Data File : VV020341.D
Acq On : 17 Feb 2021 12:44
Operator : SY/MD
Sample : VIBLK63
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021721\
Data File : VV020341.D
Acq On : 17 Feb 2021 12:44
Operator : SY/MD
Sample : VIBLK63
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
