
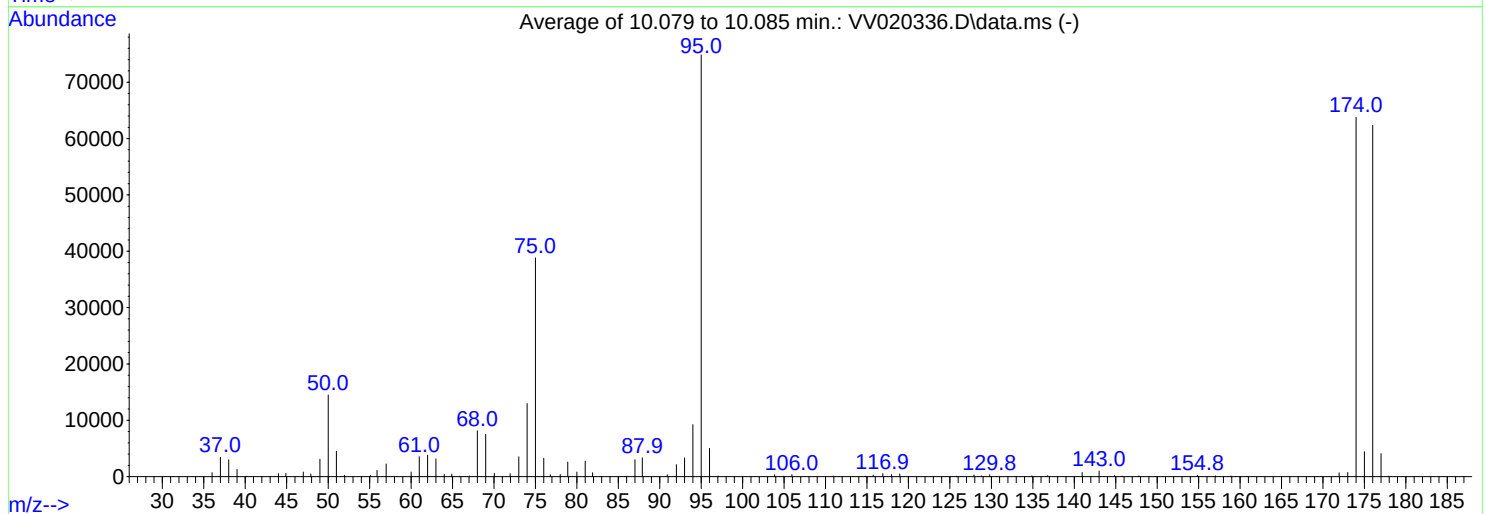


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021721\
Data File : VV020336.D
Acq On : 17 Feb 2021 08:54
Operator : SY/MD
Sample : BFB93
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB93

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Title : VOC Analysis
Last Update : Thu Feb 18 00:34:19 2021

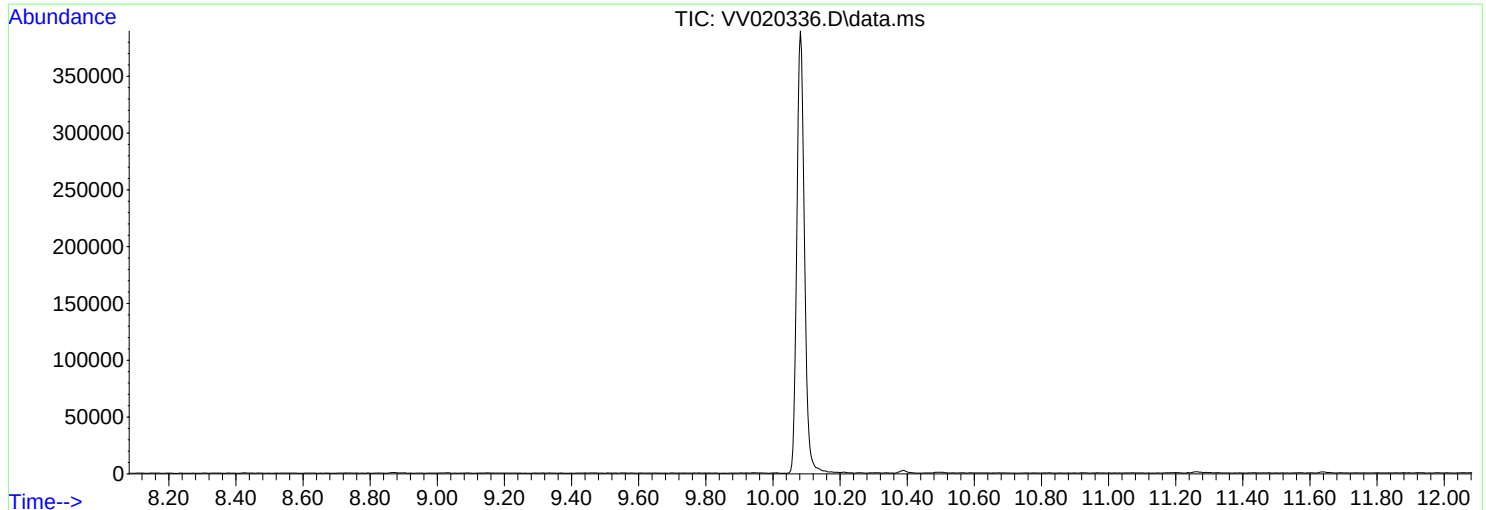

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	14480	PASS
75	95	30	80	51.9	38824	PASS
95	95	100	100	100.0	74853	PASS
96	95	5	9	6.7	5021	PASS
173	174	0.00	2	1.2	742	PASS
174	95	50	120	85.2	63763	PASS
175	174	5	9	7.0	4439	PASS
176	174	95	101	97.7	62317	PASS
177	176	5	9	6.6	4097	PASS

m/z	Abundance
36.00	658.0
37.00	3442.0
38.00	2952.0
39.00	1347.0
40.20	239.0
44.00	959.0
44.90	560.0
47.00	844.0
47.90	428.0
49.00	3032.0
50.00	14100.0
51.00	4321.0
51.90	262.0
55.10	193.0
55.90	1053.0
57.00	2200.0
58.20	110.0
60.00	823.0
61.00	3425.0
62.00	3774.0
63.00	3196.0
64.10	393.0
64.90	454.0
65.90	117.0
66.80	195.0
68.00	8094.0
69.00	7503.0
70.00	553.0
71.90	486.0
73.00	3491.0
74.00	13062.0
75.00	38760.0
76.00	3270.0
78.00	432.0
78.90	2631.0
80.00	868.0
81.00	2656.0
81.90	656.0
82.90	102.0
87.00	2869.0
87.90	3353.0
90.80	338.0
92.00	2097.0
93.00	3196.0
94.00	9176.0
95.00	74352.0
96.00	4893.0
97.00	134.0
103.90	355.0
106.00	370.0
111.00	127.0
114.80	120.0
115.70	284.0
116.90	585.0
117.90	394.0
119.00	448.0
127.90	262.0
128.70	115.0
129.80	357.0
134.90	130.0
136.80	182.0
140.90	706.0
143.00	907.0
144.90	239.0
145.80	106.0
147.80	173.0
149.80	102.0
154.80	227.0
157.00	129.0
158.90	116.0
172.00	587.0
173.00	648.0
174.00	61944.0
175.00	4361.0
176.00	60112.0
177.00	4006.0
178.00	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

m/z	Abundance
36.00	765.0
37.00	3555.0
38.00	3125.0
39.00	1275.0
39.90	266.0
44.00	1030.0
44.90	572.0
47.00	862.0
47.90	499.0
49.00	3193.0
50.00	15003.0
51.00	4678.0
51.90	223.0
55.10	211.0
55.90	1158.0
57.00	2334.0
60.00	870.0
61.00	3663.0
62.00	3909.0
63.00	3288.0
64.00	398.0
64.90	483.0
65.90	107.0
67.00	160.0
68.00	8467.0
69.00	7730.0
70.10	629.0
72.00	573.0
73.00	3614.0
74.00	13293.0
75.00	40088.0
76.00	3405.0
76.80	523.0
78.00	367.0
78.90	2690.0
80.00	842.0
81.00	2812.0
81.90	730.0
85.80	117.0
86.00	116.0
87.00	3103.0
87.90	3405.0
90.90	343.0
92.00	2204.0
93.00	3450.0
94.00	9537.0
95.00	77424.0
96.00	5158.0
97.00	129.0
103.80	346.0
104.90	126.0
106.00	410.0
111.00	136.0
114.80	129.0
115.80	293.0
116.90	557.0
117.90	382.0
118.90	503.0
125.80	108.0
127.90	302.0
128.80	132.0
129.80	357.0
134.90	146.0
136.80	190.0
140.90	758.0
142.00	106.0
143.00	1026.0
144.80	201.0
145.70	117.0
147.80	149.0
154.80	235.0
157.00	158.0
158.90	128.0
171.90	681.0
173.00	753.0
174.00	65768.0
175.00	4554.0
176.00	64336.0
177.00	4267.0
177.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

m/z	Abundance
36.00	759.0
37.00	3295.0
38.00	2904.0
39.00	1187.0
39.90	311.0
44.00	977.0
44.90	561.0
47.00	807.0
47.90	492.0
49.00	3031.0
50.00	14336.0
51.00	4475.0
52.00	212.0
55.10	192.0
55.90	1124.0
57.00	2217.0
60.00	769.0
61.00	3547.0
62.00	3772.0
63.00	2983.0
63.90	421.0
64.90	443.0
67.10	159.0
68.00	7849.0
69.00	7253.0
70.10	637.0
72.00	596.0
73.00	3434.0
74.00	12585.0
75.00	37624.0
76.00	3131.0
76.80	535.0
78.00	275.0
78.90	2465.0
80.00	780.0
81.00	2768.0
81.90	693.0
86.10	140.0
87.00	3077.0
87.90	3180.0
91.00	335.0
92.00	2119.0
93.00	3352.0
94.00	8945.0
95.00	72784.0
96.00	5011.0
97.10	126.0
103.80	359.0
104.90	149.0
105.90	366.0
110.90	126.0
115.80	308.0
116.90	485.0
118.00	347.0
118.90	525.0
125.80	107.0
127.90	335.0
128.90	156.0
129.80	279.0
130.60	112.0
134.90	163.0
136.80	156.0
141.00	780.0
143.00	1043.0
144.80	163.0
145.70	119.0
147.80	155.0
154.90	225.0
157.10	170.0
158.90	126.0
160.80	100.0
171.90	749.0
173.00	826.0
174.00	63576.0
175.00	4401.0
176.00	62504.0
177.00	4017.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

m/z	Abundance
40.00	222.0
44.00	460.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93