

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021820\
 Data File : VV014602.D
 Acq On : 18 Feb 2020 11:14
 Operator : SY/MD
 Sample : VV0218WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK72

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.582	146	153	166	rBV	53340	64194	7.36%	0.987%
2	2.042	293	296	298	rBV	404	172	0.02%	0.003%
3	2.132	315	324	339	rVB	118732	170457	19.54%	2.620%
4	2.521	442	445	446	rBV2	533	316	0.04%	0.005%
5	2.708	502	503	507	rBV	351	267	0.03%	0.004%
6	2.775	523	524	526	rBV	237	70	0.01%	0.001%
7	2.872	551	554	557	rVB2	420	276	0.03%	0.004%
8	2.907	564	565	568	rBV2	250	96	0.01%	0.001%
9	2.942	573	576	577	rBV	654	278	0.03%	0.004%
10	3.109	627	628	631	rBV	205	106	0.01%	0.002%
11	3.129	631	634	635	rBV	229	102	0.01%	0.002%
12	3.167	645	646	647	rBV	367	104	0.01%	0.002%
13	3.193	653	654	656	rBV	318	118	0.01%	0.002%
14	3.219	660	662	664	rBV2	408	153	0.02%	0.002%
15	3.299	685	687	689	rVB2	391	126	0.01%	0.002%
16	3.405	717	720	721	rBV2	152	79	0.01%	0.001%
17	3.618	782	786	788	rBV2	280	197	0.02%	0.003%
18	3.659	796	799	800	rBV	245	97	0.01%	0.001%
19	3.679	800	805	808	rVB3	395	350	0.04%	0.005%
20	3.704	808	813	816	rBV2	396	264	0.03%	0.004%
21	3.717	816	817	819	rBV	122	56	0.01%	0.001%
22	3.775	833	835	836	rBV	223	80	0.01%	0.001%
23	3.801	842	843	844	rBB	185	36	0.00%	0.001%
24	3.820	848	849	850	rBV	243	66	0.01%	0.001%
25	3.846	854	857	858	rBV	340	184	0.02%	0.003%
26	3.923	871	881	910	rBV	64305	167836	19.23%	2.579%
27	4.302	998	999	1002	rBV	421	208	0.02%	0.003%
28	4.589	1086	1088	1091	rBV3	563	252	0.03%	0.004%
29	4.666	1107	1112	1113	rBV	552	440	0.05%	0.007%
30	4.743	1133	1136	1139	rBV4	343	352	0.04%	0.005%
31	4.852	1168	1170	1171	rBV4	176	77	0.01%	0.001%
32	4.920	1188	1191	1192	rBV2	350	196	0.02%	0.003%
33	4.945	1198	1199	1201	rVB2	268	82	0.01%	0.001%
34	5.003	1216	1217	1219	rBV2	288	146	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021820\
 Data File : VV014602.D
 Acq On : 18 Feb 2020 11:14
 Operator : SY/MD
 Sample : VV0218WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK72

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

35	5.093	1228	1245	1272	rBV2	347273	872567	100.00%	13.409%
36	5.347	1321	1324	1327	rBV2	665	396	0.05%	0.006%
37	5.425	1346	1348	1352	rBV2	372	250	0.03%	0.004%
38	5.457	1356	1358	1361	rBV3	822	351	0.04%	0.005%
39	5.508	1371	1374	1376	rBV	363	178	0.02%	0.003%
40	5.527	1376	1380	1383	rBV2	630	613	0.07%	0.009%
41	5.572	1392	1394	1396	rVB2	277	78	0.01%	0.001%
42	5.582	1396	1397	1400	rBV	206	113	0.01%	0.002%
43	5.662	1406	1422	1445	rBV	321907	641499	73.52%	9.858%
44	6.113	1548	1562	1590	rBV	194444	399318	45.76%	6.137%
45	6.347	1633	1635	1636	rVB	320	123	0.01%	0.002%
46	6.373	1640	1643	1645	rBV	422	228	0.03%	0.004%
47	6.437	1660	1663	1665	rBV	202	143	0.02%	0.002%
48	6.611	1716	1717	1719	rVB	230	45	0.01%	0.001%
49	6.643	1725	1727	1729	rBV	247	124	0.01%	0.002%
50	6.807	1774	1778	1779	rBV2	259	152	0.02%	0.002%
51	6.932	1816	1817	1822	rBV2	283	140	0.02%	0.002%
52	7.026	1835	1846	1864	rBV	124130	219818	25.19%	3.378%
53	7.357	1935	1949	1967	rBV	430662	745144	85.40%	11.451%
54	7.659	2030	2043	2064	rBV	86433	150781	17.28%	2.317%
55	8.048	2162	2164	2165	rBV	265	87	0.01%	0.001%
56	8.064	2167	2169	2173	rVB	444	274	0.03%	0.004%
57	8.087	2173	2176	2178	rBV	476	239	0.03%	0.004%
58	8.125	2178	2188	2223	rBV	182054	385212	44.15%	5.920%
59	8.659	2353	2354	2355	rBV	171	47	0.01%	0.001%
60	8.669	2355	2357	2360	rVB2	300	100	0.01%	0.002%
61	8.691	2360	2364	2365	rBV	331	225	0.03%	0.003%
62	8.891	2415	2426	2450	rBV	476346	766879	87.89%	11.785%
63	9.129	2497	2500	2501	rBV2	419	235	0.03%	0.004%
64	9.280	2546	2547	2549	rBV	247	79	0.01%	0.001%
65	9.530	2622	2625	2627	rBV	350	147	0.02%	0.002%
66	9.579	2634	2640	2645	rBV2	698	764	0.09%	0.012%
67	9.826	2715	2717	2719	rVV	549	153	0.02%	0.002%
68	9.836	2719	2720	2722	rVB	325	99	0.01%	0.002%
69	9.907	2740	2742	2743	rBV	288	129	0.01%	0.002%
70	10.006	2772	2773	2774	rBV	238	75	0.01%	0.001%
71	10.087	2796	2798	2799	rBV	129	38	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021820\
Data File : VV014602.D
Acq On : 18 Feb 2020 11:14
Operator : SY/MD
Sample : VV0218WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK72

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Title : VOC Analysis

72	10.125	2805	2810	2816	rBV2	437	439	0.05%	0.007%
73	10.151	2816	2818	2820	rBV	242	103	0.01%	0.002%
74	10.254	2837	2850	2872	rBV	283391	444627	50.96%	6.833%
75	11.003	3080	3083	3084	rBV2	221	125	0.01%	0.002%
76	11.289	3160	3172	3194	rBV	486780	771240	88.39%	11.852%
77	11.543	3249	3251	3254	rBV	431	154	0.02%	0.002%
78	11.665	3276	3289	3312	rBV	433331	695409	79.70%	10.687%
79	12.292	3483	3484	3485	rBV	196	58	0.01%	0.001%
80	12.350	3499	3502	3504	rBV2	376	270	0.03%	0.004%


Sum of corrected areas: 6507101

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV021820\
Data File : VV014602.D
Acq On : 18 Feb 2020 11:14
Operator : SY/MD
Sample : VV0218WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK72

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

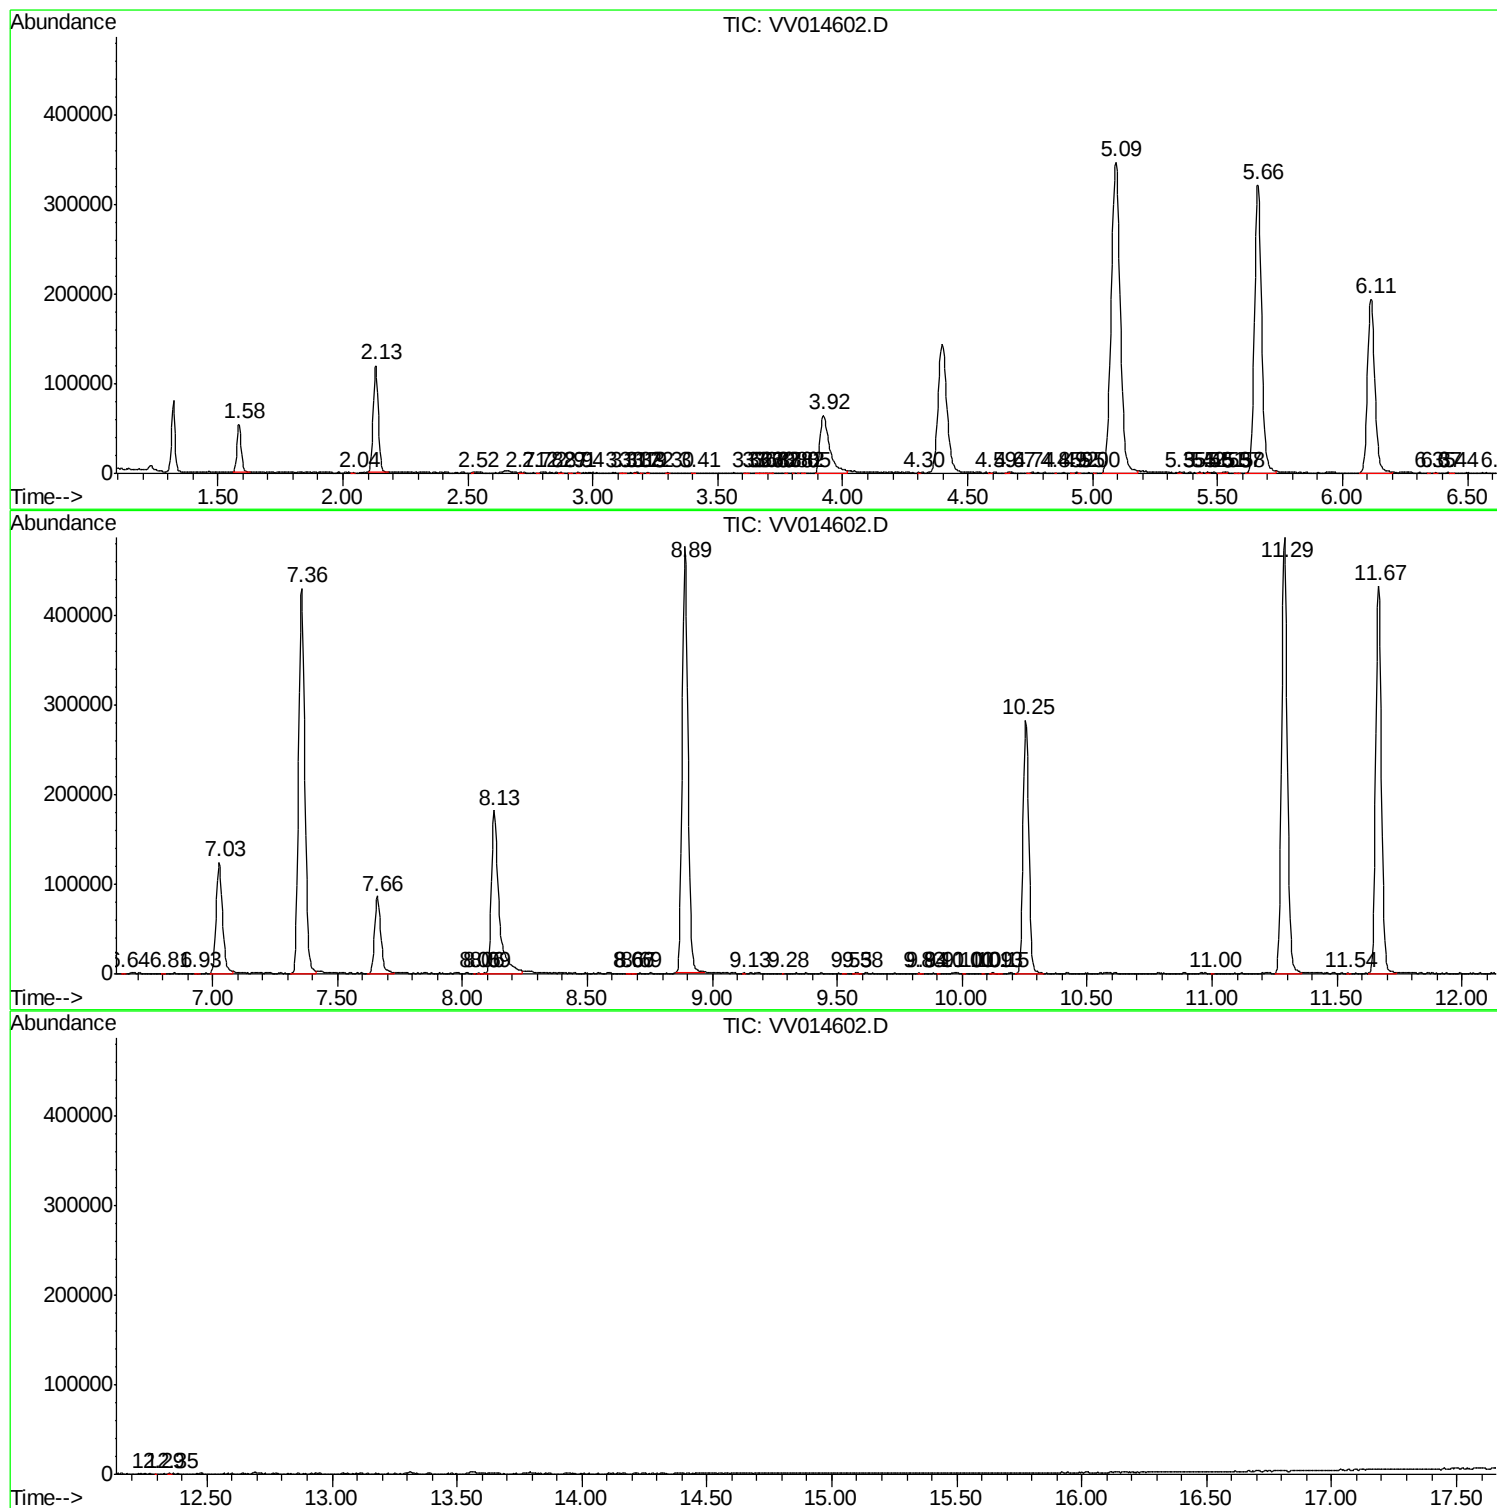

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV021820\
Data File : VV014602.D
Acq On : 18 Feb 2020 11:14
Operator : SY/MD
Sample : VV0218WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK72

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV021820\
Data File : VV014602.D
Acq On : 18 Feb 2020 11:14
Operator : SY/MD
Sample : VV0218WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK72

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc