


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV021820\
 Data File : VV014600.D
 Acq On : 18 Feb 2020 09:39
 Operator : SY/MD
 Sample : BFB92
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB92

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis
 Last Update : Wed Feb 19 01:18:31 2020

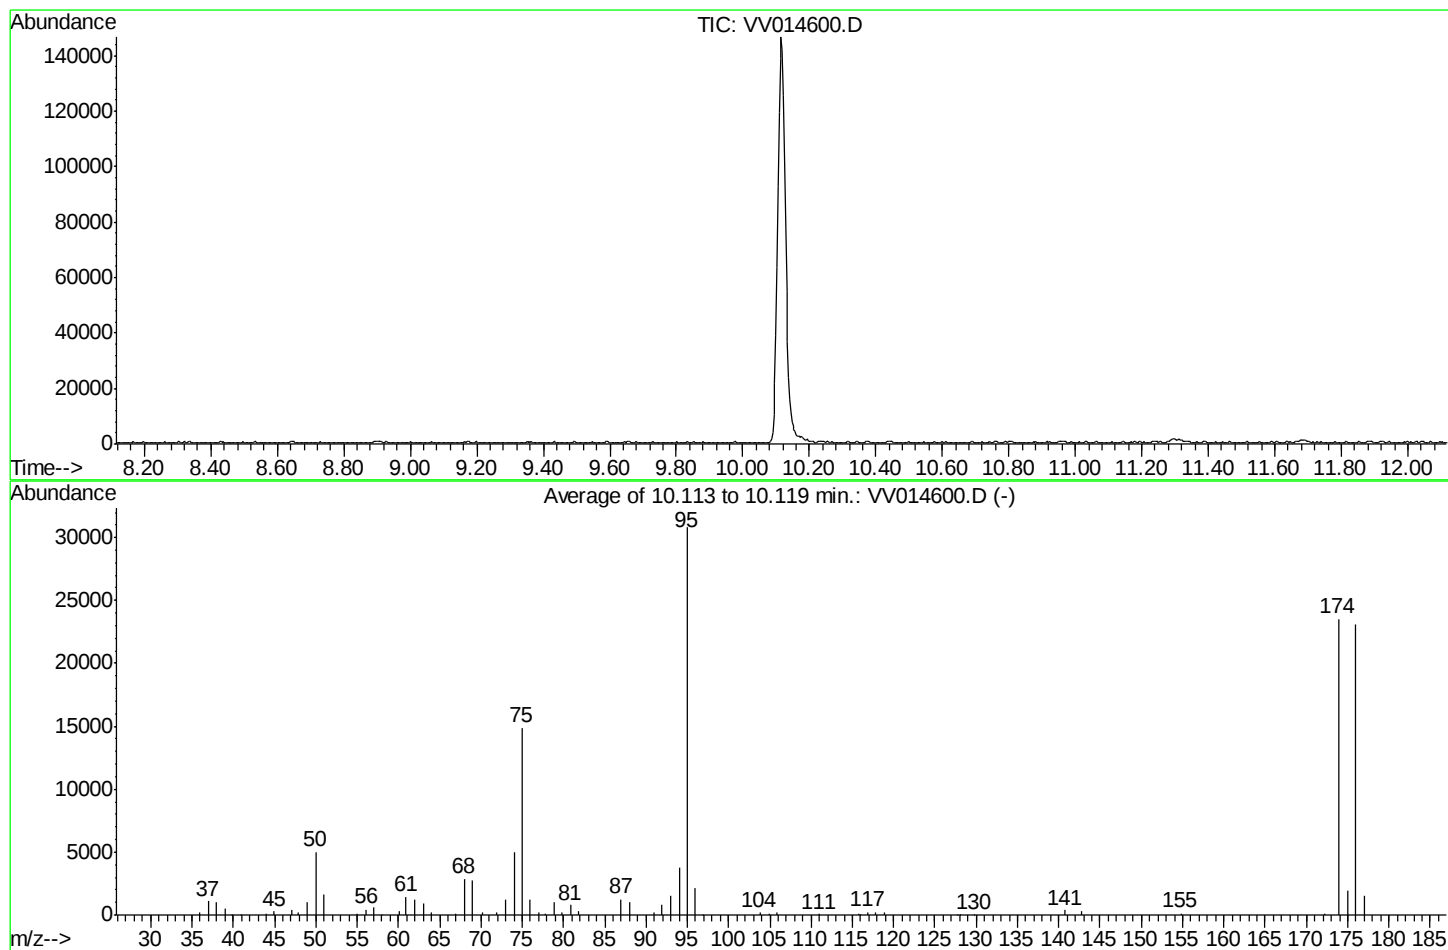

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	5025	PASS
75	95	30	80	48.3	14876	PASS
95	95	100	100	100.0	30813	PASS
96	95	5	9	7.0	2172	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.4	23530	PASS
175	174	5	9	8.1	1911	PASS
176	174	95	101	98.2	23112	PASS
177	176	5	9	6.4	1483	PASS

m/z	Abundance
36.00	251.0
37.00	1092.0
38.00	1036.0
39.00	443.0
39.80	280.0
40.90	101.0
43.90	382.0
44.90	281.0
47.00	383.0
47.80	230.0
49.00	1105.0
50.00	5178.0
51.00	1655.0
55.00	134.0
56.10	441.0
57.00	605.0
57.90	108.0
60.10	291.0
60.90	1435.0
62.00	1220.0
63.00	875.0
64.00	158.0
67.00	117.0
68.00	2858.0
69.00	2783.0
70.20	154.0
71.90	201.0
72.90	1157.0
74.00	4810.0
75.00	14764.0
76.00	1247.0
77.00	185.0
77.80	158.0
78.90	1077.0
79.80	253.0
80.80	830.0
81.80	308.0
87.00	1113.0
87.90	1022.0
91.00	199.0
91.90	816.0
93.00	1387.0
94.00	3694.0
95.00	30336.0
96.00	2018.0
103.80	176.0
104.90	103.0
105.90	168.0
116.00	129.0
116.80	226.0
117.80	182.0
118.80	183.0
128.00	114.0
140.80	347.0
142.80	304.0
154.80	153.0
173.90	22592.0
175.00	1872.0
175.90	21864.0
177.00	1403.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

m/z	Abundance
35.90	249.0
37.00	1100.0
37.90	1034.0
38.90	529.0
39.80	263.0
43.90	443.0
45.00	326.0
47.10	384.0
47.80	214.0
49.00	1075.0
50.00	5118.0
51.00	1629.0
55.00	146.0
56.10	430.0
57.00	678.0
60.10	303.0
60.90	1534.0
62.00	1255.0
63.00	941.0
64.00	166.0
67.00	153.0
68.00	2946.0
69.00	2866.0
70.20	154.0
72.00	189.0
73.00	1209.0
74.00	5132.0
75.00	15328.0
76.00	1290.0
77.00	258.0
77.80	111.0
78.90	1076.0
79.90	260.0
80.90	795.0
81.80	310.0
87.00	1280.0
88.00	1045.0
91.00	188.0
91.90	840.0
92.90	1590.0
94.00	3918.0
95.00	31736.0
96.00	2232.0
103.80	199.0
104.90	112.0
105.80	174.0
111.00	123.0
115.70	145.0
116.90	233.0
117.80	174.0
118.90	153.0
140.80	389.0
142.80	333.0
154.80	152.0
172.20	129.0
173.90	24272.0
174.90	2002.0
175.90	23896.0
176.90	1520.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

m/z	Abundance
35.80	249.0
37.00	1074.0
37.90	936.0
38.90	539.0
39.90	215.0
44.00	460.0
44.90	301.0
47.10	329.0
47.90	184.0
48.90	973.0
50.00	4781.0
51.00	1519.0
55.00	146.0
56.10	408.0
57.00	689.0
60.00	307.0
60.90	1421.0
62.00	1204.0
63.00	914.0
64.00	157.0
67.00	147.0
68.00	2825.0
69.00	2745.0
70.10	173.0
72.00	195.0
73.00	1256.0
74.00	5084.0
75.00	14537.0
76.00	1275.0
77.00	290.0
78.90	890.0
79.90	260.0
80.90	797.0
81.80	270.0
87.00	1333.0
87.90	1045.0
91.00	117.0
91.90	768.0
92.90	1478.0
94.00	3780.0
95.00	30368.0
96.00	2266.0
96.80	117.0
103.80	192.0
105.80	158.0
111.00	105.0
115.70	178.0
117.00	243.0
117.80	135.0
118.80	151.0
127.70	110.0
129.80	119.0
140.80	386.0
142.70	350.0
154.90	132.0
172.20	143.0
173.90	23728.0
174.90	1861.0
175.90	23576.0
176.90	1526.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

Scan 2795 (10.077 min): VV014600.D
BFB92

m/z	Abundance
39.90	218.0
44.10	281.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92