


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV021920\
 Data File : VV014605.D
 Acq On : 19 Feb 2020 13:24
 Operator : SY/MD
 Sample : BFB38
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB701

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVTR021920WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Feb 20 02:48:04 2020

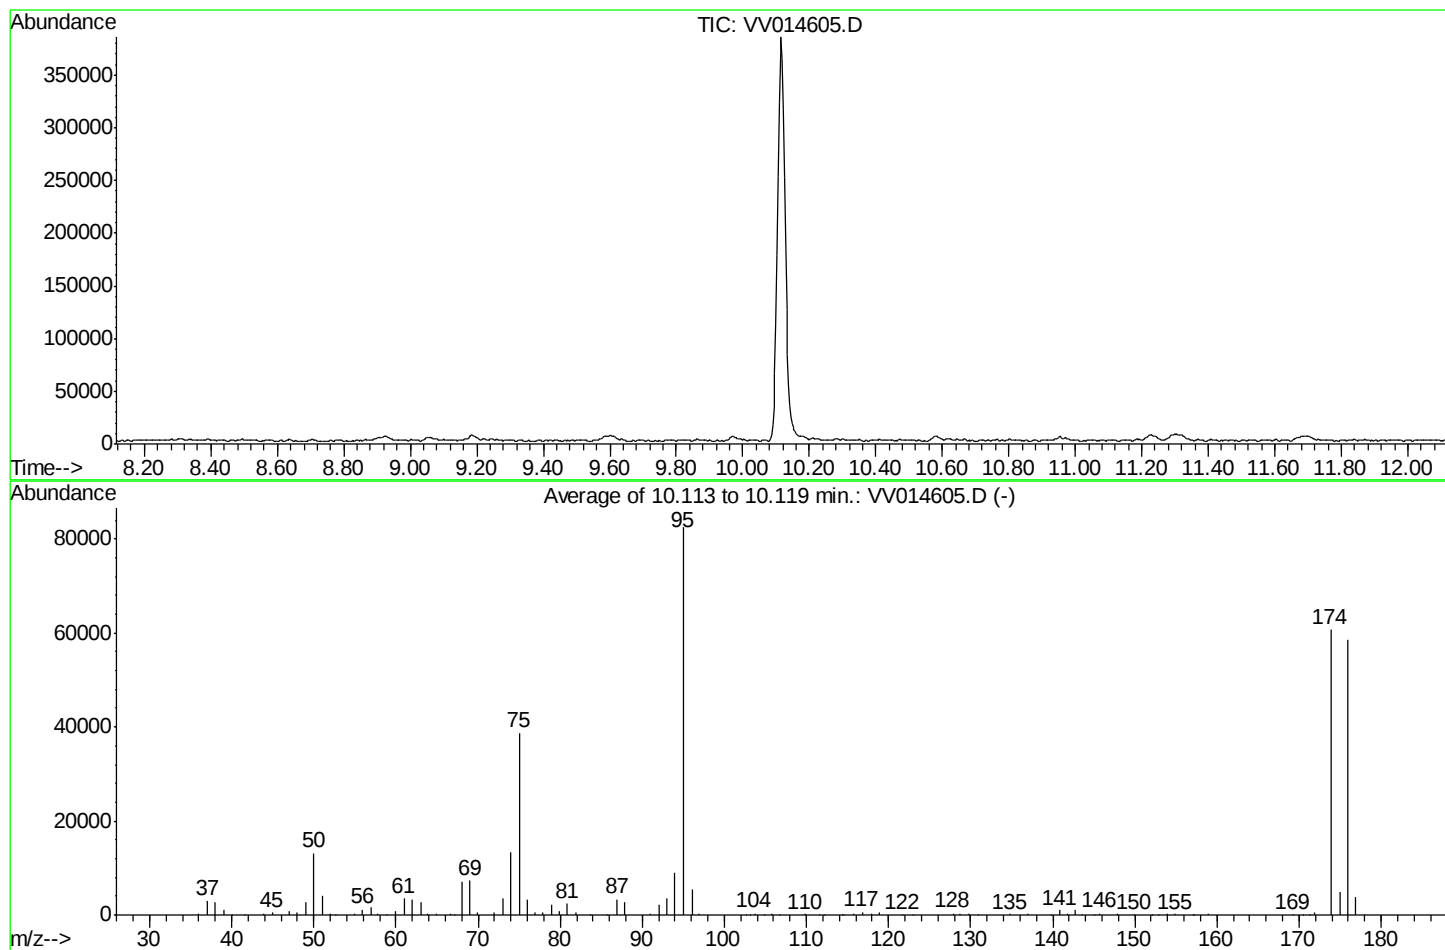

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	13180	PASS
75	95	30	80	47.0	38797	PASS
95	95	100	100	100.0	82488	PASS
96	95	5	9	6.6	5442	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.6	60728	PASS
175	174	5	9	8.0	4846	PASS
176	174	95	105	96.5	58602	PASS
177	176	5	10	6.4	3728	PASS

m/z	Abundance
35.90	555.0
37.00	3315.0
38.00	2866.0
39.00	1276.0
40.00	480.0
40.60	120.0
41.60	141.0
44.00	868.0
45.00	664.0
46.90	798.0
48.00	483.0
49.00	2658.0
50.00	13401.0
51.00	3956.0
51.90	238.0
55.10	297.0
55.90	1131.0
57.00	1630.0
57.80	167.0
59.90	722.0
61.00	3706.0
62.00	3588.0
63.00	2853.0
63.80	253.0
64.80	210.0
66.60	216.0
67.10	216.0
68.00	7004.0
69.00	7230.0
69.90	501.0
72.00	533.0
73.00	3601.0
74.00	13397.0
75.00	38904.0
76.00	3198.0
76.90	510.0
77.80	507.0
78.90	2485.0
79.90	699.0
80.90	2420.0
81.90	514.0
83.60	112.0
85.70	203.0
87.00	3479.0
87.90	3088.0
90.90	283.0
92.00	2017.0
93.00	3700.0
94.00	8970.0
95.00	81936.0
96.00	5660.0
96.90	295.0
102.60	135.0
103.70	385.0
104.80	131.0
105.80	363.0
106.70	117.0
109.80	209.0
111.60	108.0
114.30	106.0
114.50	103.0
115.70	171.0
116.80	551.0
117.90	363.0
118.90	386.0
127.90	416.0
128.70	167.0
129.90	398.0
130.90	109.0
134.90	211.0
137.00	203.0
139.70	116.0
140.90	990.0
141.80	124.0
142.80	950.0
145.00	164.0
145.80	300.0
147.70	273.0
150.00	131.0
152.10	123.0
153.90	151.0
155.00	294.0
157.30	107.0
158.90	178.0
169.30	141.0
171.90	413.0
173.90	59200.0
174.90	4986.0
175.90	56680.0
177.00	3747.0
177.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB701

m/z	Abundance
35.90	524.0
37.00	3145.0
38.00	2937.0
39.00	1200.0
40.00	442.0
40.70	134.0
44.00	837.0
44.90	675.0
47.00	849.0
48.00	530.0
49.00	2770.0
50.00	13612.0
51.00	4141.0
52.00	231.0
52.60	109.0
54.20	109.0
55.10	350.0
55.90	1183.0
57.00	1882.0
57.80	190.0
60.00	798.0
61.00	3622.0
62.00	3339.0
63.00	2814.0
63.80	268.0
64.80	198.0
66.60	234.0
67.10	265.0
68.00	7071.0
69.00	7524.0
69.90	541.0
72.00	464.0
73.00	3582.0
74.00	13695.0
75.00	40072.0
76.10	3353.0
76.90	588.0
77.80	441.0
78.90	2355.0
79.90	768.0
80.90	2500.0
82.00	584.0
83.70	109.0
85.70	158.0
86.90	3375.0
87.90	3025.0
91.00	306.0
92.00	2279.0
93.00	3815.0
94.00	9439.0
95.00	85008.0
96.00	5561.0
96.90	229.0
102.60	117.0
103.70	401.0
104.90	159.0
105.90	375.0
106.80	116.0
109.80	194.0
111.60	122.0
112.20	109.0
115.80	206.0
116.80	633.0
118.00	323.0
118.80	478.0
121.70	109.0
127.90	368.0
128.70	189.0
129.90	316.0
131.00	117.0
134.80	205.0
137.00	214.0
140.90	1056.0
141.90	166.0
142.80	1062.0
143.50	109.0
145.10	141.0
145.80	322.0
147.80	261.0
149.90	136.0
152.10	121.0
152.80	130.0
153.90	203.0
155.00	274.0
157.00	116.0
158.90	169.0
169.30	120.0
171.30	137.0
171.90	435.0
173.90	62536.0
175.00	5090.0
175.90	60632.0

Instrument :
MSVOA_V
ClientSampleId :
BFB701

176.903864.0

178.00119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB701

m/z	Abundance
36.00	507.0
37.10	2942.0
38.00	2820.0
39.10	1108.0
39.90	388.0
43.30	159.0
44.00	756.0
44.90	670.0
47.10	971.0
47.90	494.0
49.00	2619.0
50.00	12527.0
51.00	3943.0
52.00	261.0
52.60	118.0
54.20	102.0
55.00	294.0
55.90	1082.0
57.00	1871.0
57.80	153.0
58.90	123.0
60.00	742.0
61.00	3306.0
62.00	2877.0
63.00	2478.0
63.90	284.0
64.90	190.0
67.10	280.0
68.00	6918.0
69.00	7153.0
70.00	587.0
72.00	371.0
73.00	3281.0
74.00	12764.0
75.00	37416.0
76.10	3134.0
76.90	661.0
77.90	321.0
78.90	2120.0
79.90	748.0
80.90	2316.0
82.00	561.0
86.90	2978.0
87.90	2673.0
91.00	322.0
92.00	2332.0
93.00	3450.0
94.00	8935.0
95.00	80520.0
96.10	5106.0
96.90	186.0
103.20	135.0
103.70	430.0
105.00	140.0
105.90	357.0
106.80	115.0
109.90	196.0
115.80	260.0
116.90	636.0
118.00	278.0
118.80	531.0
121.70	128.0
122.90	112.0
127.90	315.0
128.60	223.0
129.80	269.0
131.00	103.0
134.70	194.0
136.90	185.0
140.90	981.0
141.90	190.0
142.80	1010.0
145.10	106.0
145.70	286.0
147.90	264.0
149.90	129.0
152.10	115.0
152.80	130.0
153.90	173.0
154.80	207.0
157.00	187.0
158.90	120.0
170.50	102.0
171.20	127.0
172.00	417.0
173.90	60448.0
175.00	4462.0
175.90	58496.0
176.90	3575.0
178.00	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB701

m/z	Abundance
35.60	140.0
36.00	157.0
37.20	116.0
38.10	129.0
39.00	111.0
40.00	303.0
40.80	118.0
42.20	188.0
43.10	116.0
43.90	433.0
45.10	125.0
45.40	136.0
47.00	120.0
49.50	149.0
50.70	151.0
53.40	111.0
54.10	130.0
54.90	111.0
57.20	101.0
61.00	110.0
62.70	111.0
67.00	131.0
77.10	145.0
82.10	106.0
87.80	106.0
89.80	110.0
101.10	101.0
207.00	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB701