

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021924\
 Data File : VW034234.D
 Acq On : 19 Feb 2024 11:25
 Operator : SY/MD
 Sample : P1513-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0U25

Quant Time: Feb 19 11:47:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Feb 19 00:41:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	71519	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	66213	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	33434	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	24420	4.409	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.200%
7) Chloroethane-d5	1.532	69	21149	4.359	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.200%
11) 1,1-Dichloroethene-d2	2.060	65	11721	4.388	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.800%
20) 2-Butanone-d5	3.802	46	32637	35.084	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	70.160%
24) Chloroform-d	4.252	84	45482	4.519	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%
26) 1,2-Dichloroethane-d4	4.947	65	22741	4.835	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
32) Benzene-d6	4.960	84	85661	4.312	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.200%
36) 1,2-Dichloropropane-d6	5.989	67	23997	4.321	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.400%
41) Toluene-d8	7.243	98	79955	4.379	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.600%
43) trans-1,3-Dichloroprop...	7.561	79	8996	4.290	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.800%
46) 2-Hexanone-d5	8.030	63	25491	34.055	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	68.120%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	14062	4.177	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.600%
66) 1,2-Dichlorobenzene-d4	11.561	152	28278	4.651	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.000%
Target Compounds					Qvalue	
13) Acetone	2.127	43	5323	7.542	ug/L #	15
14) Carbon disulfide	2.243	76	3576	0.221	ug/L #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
Data File : VV034234.D
Acq On : 19 Feb 2024 11:25
Operator : SY/MD
Sample : P1513-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COU25

Quant Time: Feb 19 11:47:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Feb 19 00:41:47 2024
Response via : Initial Calibration

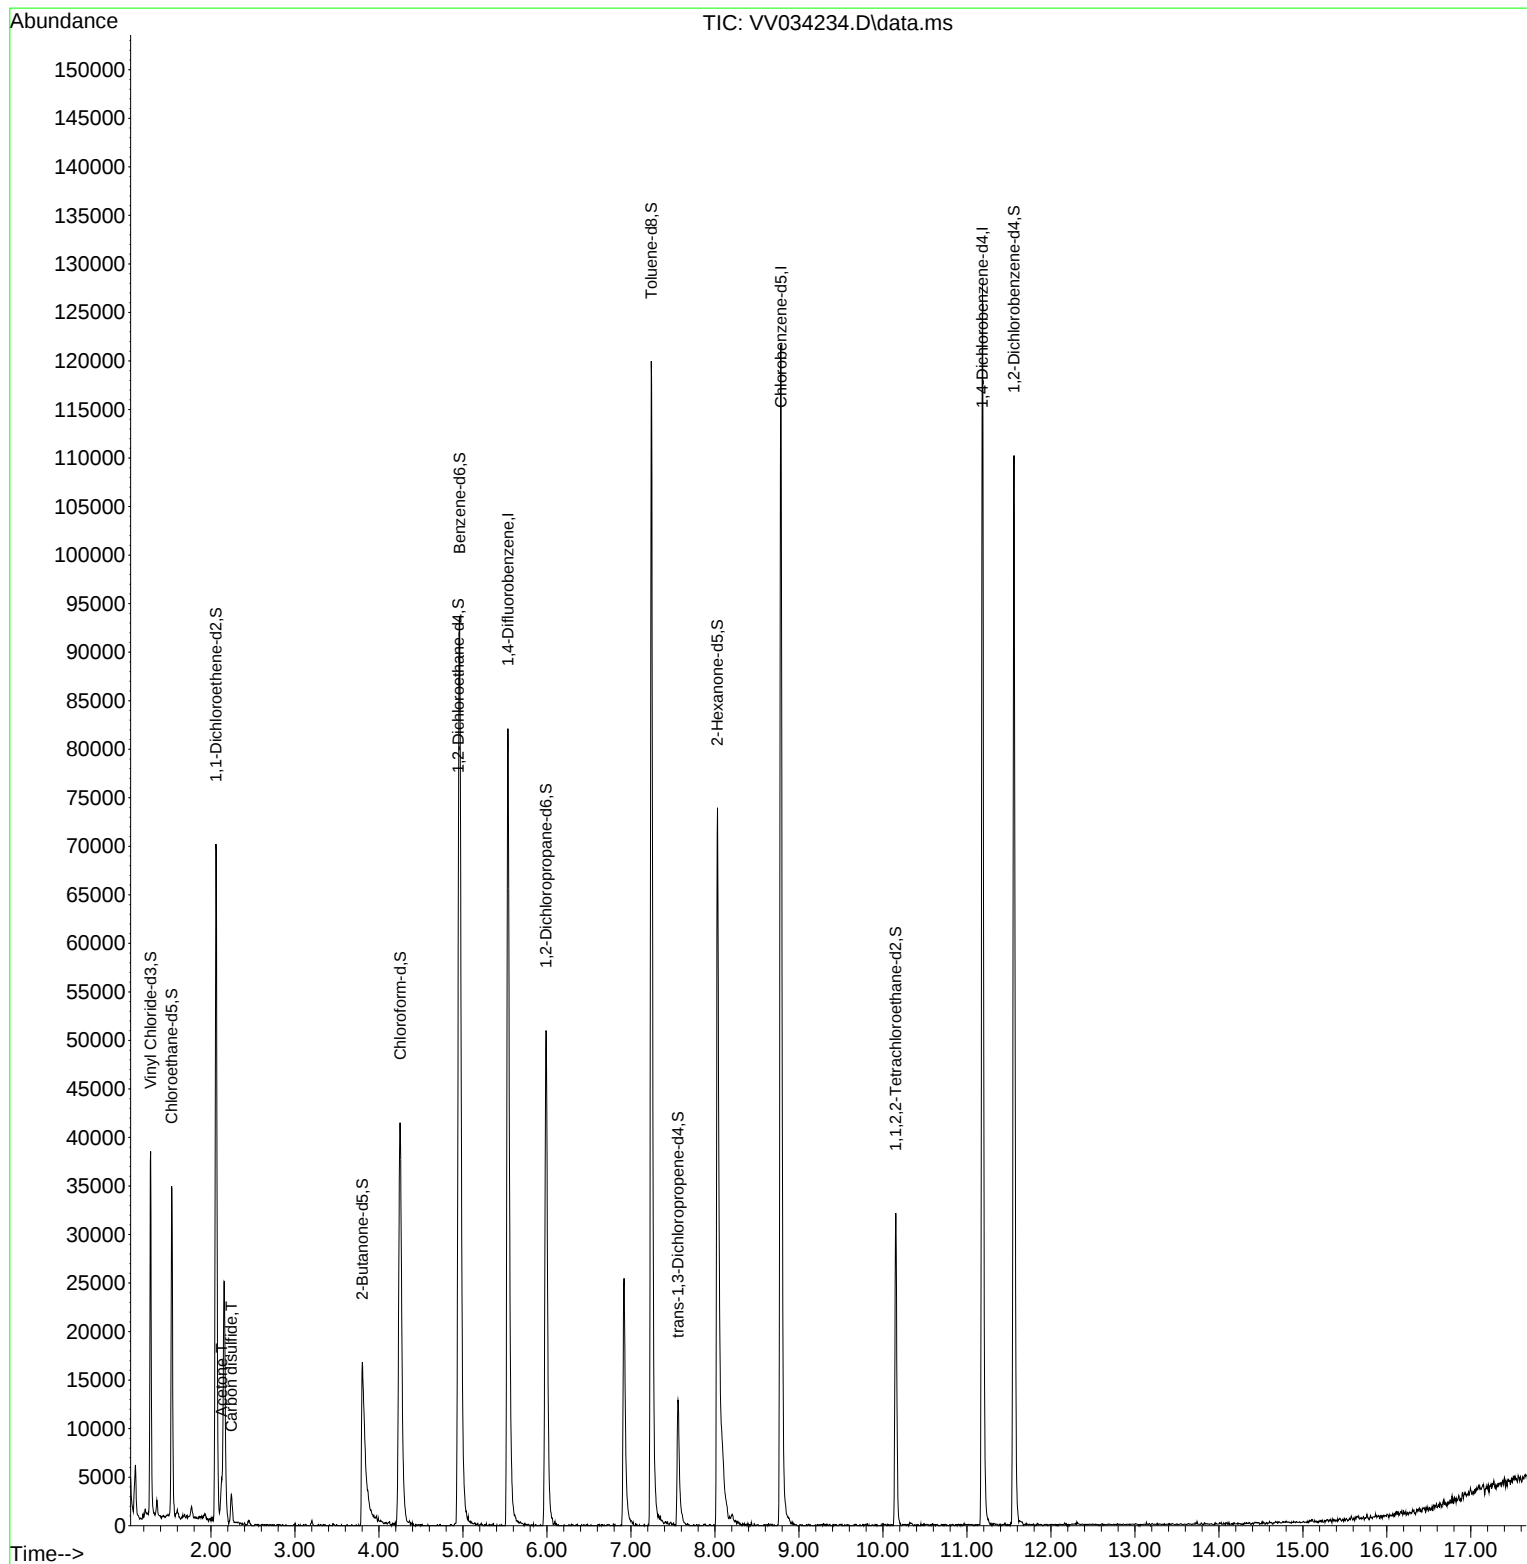

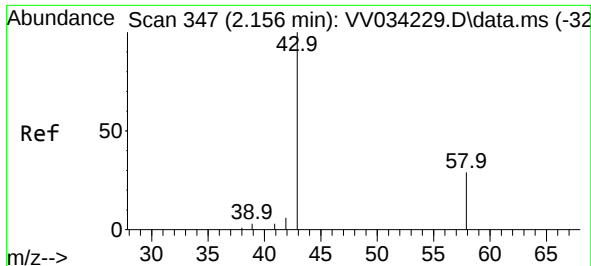

#13

Acetone

Concen: 7.542 ug/L

RT: 2.127 min Scan# 31

Delta R.T. -0.013 min

Lab File: VV034234.D

Acq: 19 Feb 2024 11:25

Instrument :

MSVOA_V

ClientSampleId :





COU25

Tgt Ion: 43 Resp: 5323

Ion Ratio Lower Upper

43 100

58 36.2 0.0 13.8#

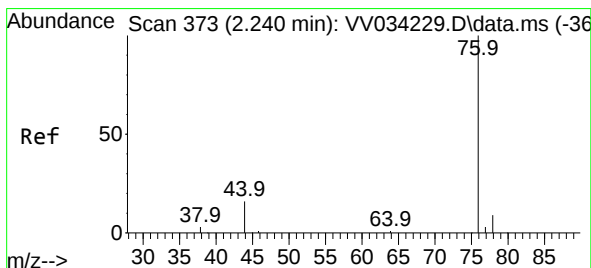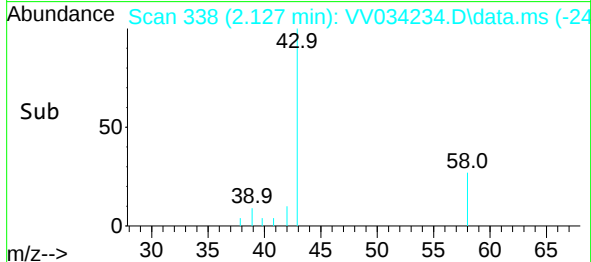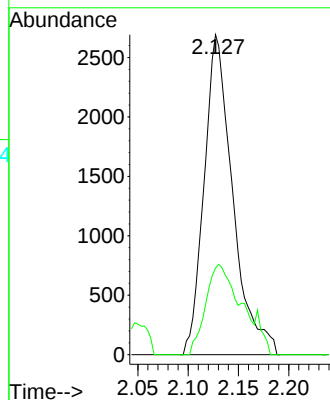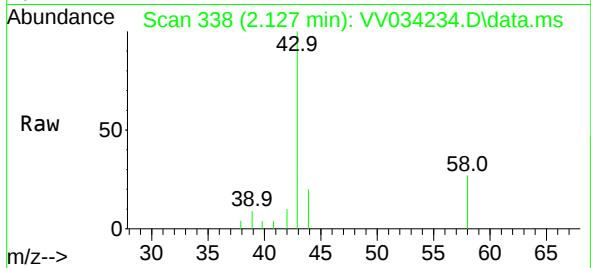

#14

Carbon disulfide

Concen: 0.221 ug/L

RT: 2.243 min Scan# 374

Delta R.T. 0.003 min

Lab File: VV034234.D

Acq: 19 Feb 2024 11:25

Tgt Ion: 76 Resp: 3576

Ion Ratio Lower Upper

76 100

78 11.4 7.5 11.3#

