

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
 Data File : VV034235.D
 Acq On : 19 Feb 2024 11:50
 Operator : SY/MD
 Sample : VIBLK324
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK324

Quant Time: Feb 20 03:27:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 20 01:47:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	75330	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	68716	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	33936	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	24413	4.185	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.600%
7) Chloroethane-d5	1.535	69	21381	4.184	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.600%
11) 1,1-Dichloroethene-d2	2.060	65	12280	4.365	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.200%
20) 2-Butanone-d5	3.805	46	38491	39.284	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	78.560%
24) Chloroform-d	4.249	84	47378	4.469	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%
26) 1,2-Dichloroethane-d4	4.944	65	24153	4.875	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.600%
32) Benzene-d6	4.960	84	89065	4.320	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
36) 1,2-Dichloropropane-d6	5.989	67	24181	4.196	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.000%
41) Toluene-d8	7.243	98	83865	4.426	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.600%
43) trans-1,3-Dichloroprop...	7.558	79	9253	4.252	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.027	63	28344	36.487	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	72.980%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	14320	4.099	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.000%
66) 1,2-Dichlorobenzene-d4	11.561	152	29108	4.716	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.400%
Target Compounds						Qvalue
16) Methylene chloride	2.449	84	885	0.175	ug/L	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
Data File : VV034235.D
Acq On : 19 Feb 2024 11:50
Operator : SY/MD
Sample : VIBLK324
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK324


Quant Time: Feb 20 03:27:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 20 01:47:35 2024
Response via : Initial Calibration

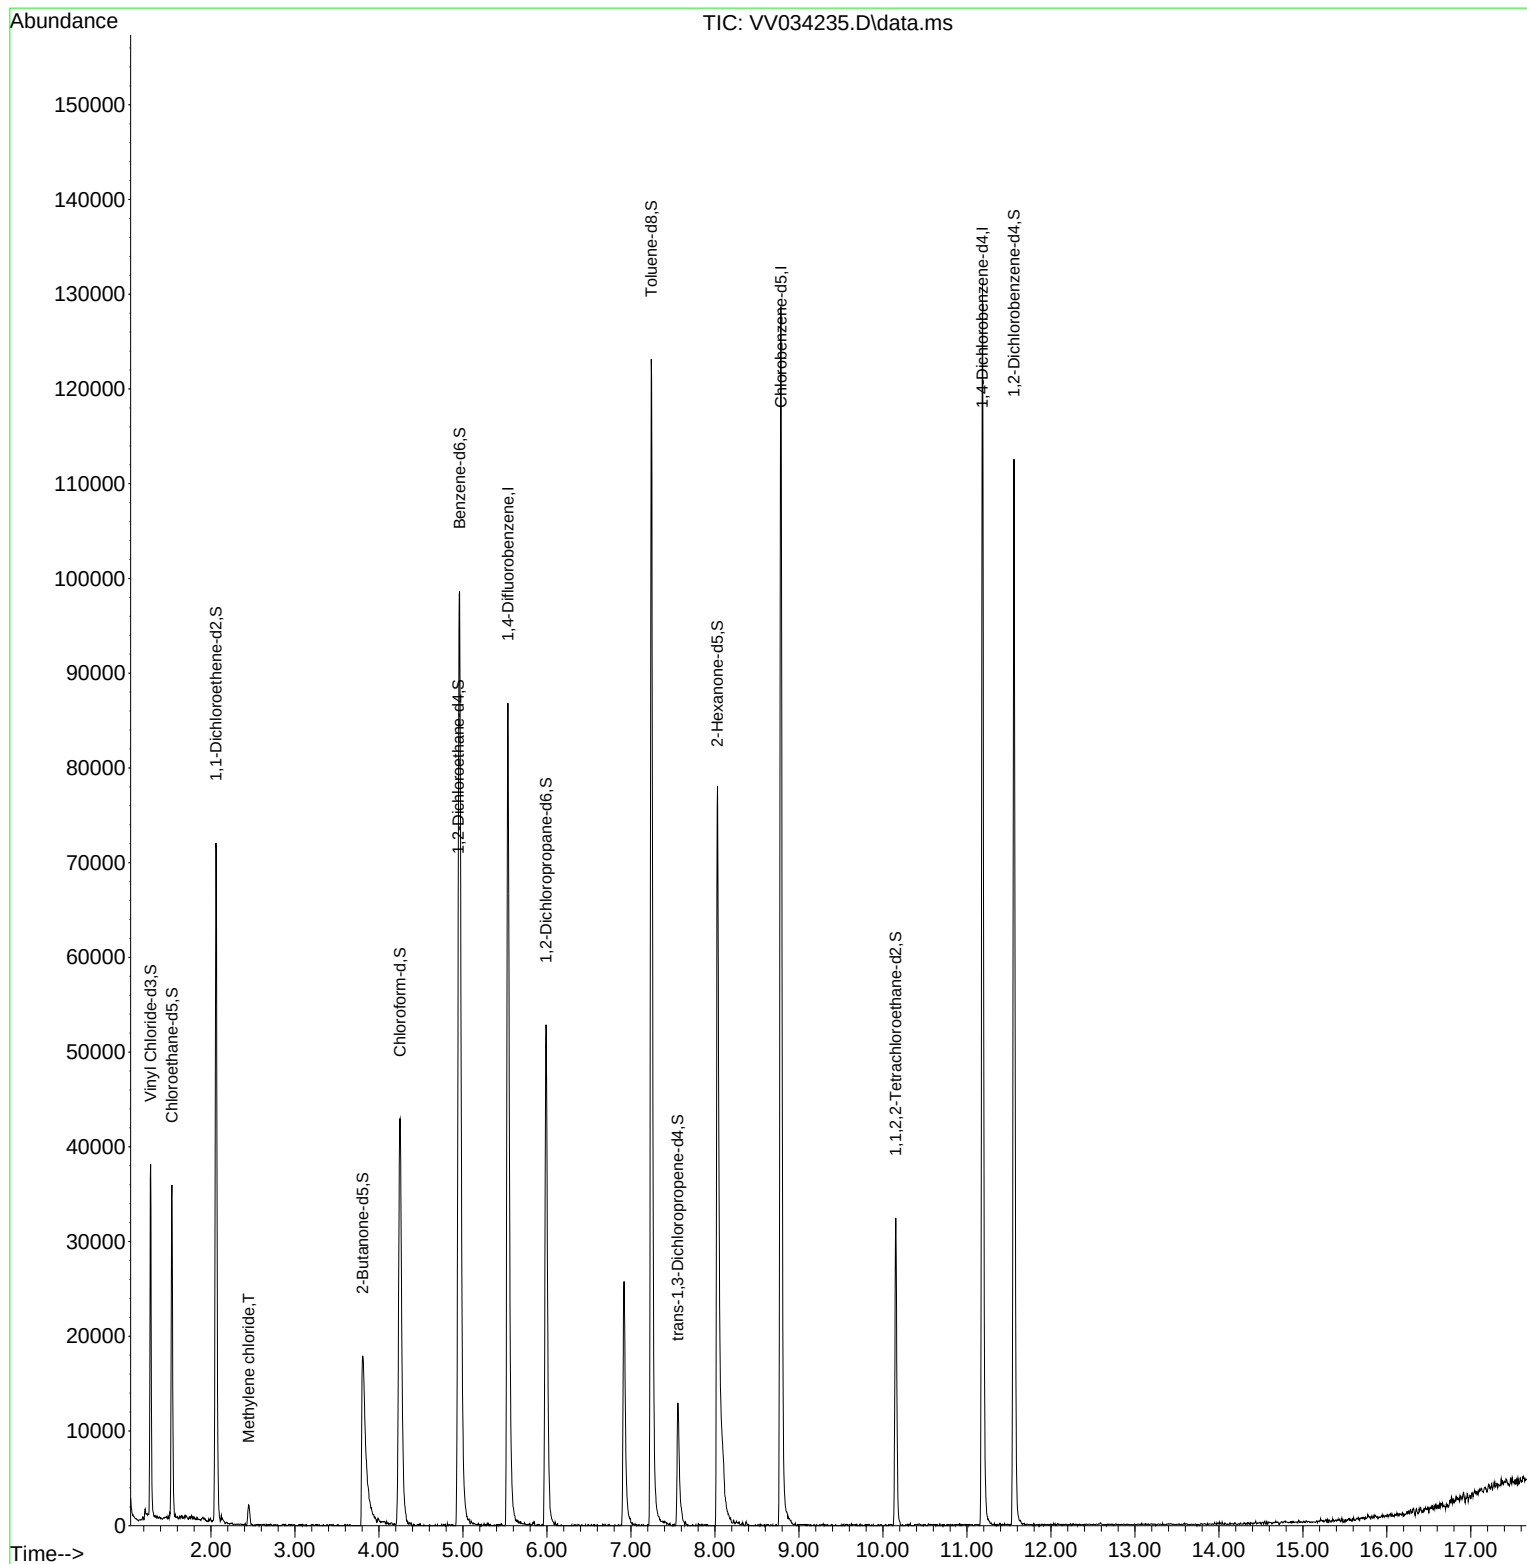

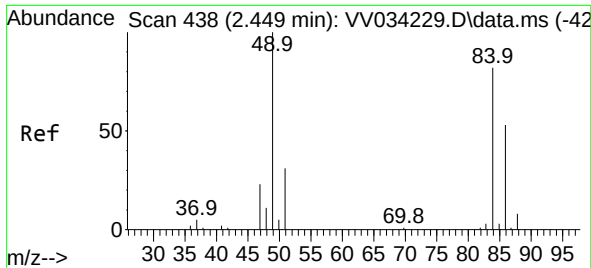

#16
Methylene chloride
Concen: 0.175 ug/L
RT: 2.449 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV034235.D
Acq: 19 Feb 2024 11:50

Instrument :
MSVOA_V
ClientSampleId :
VIBLK324

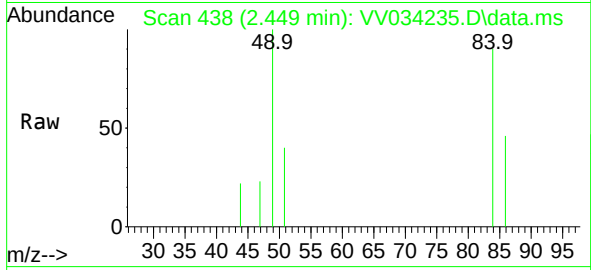

Tgt Ion:	84	Resp:	885
Ion	Ratio	Lower	Upper
84	100		
86	51.0	44.7	83.1
49	111.2	93.7	173.9

