

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
 Data File : VV034241.D
 Acq On : 19 Feb 2024 14:16
 Operator : SY/MD
 Sample : VIBLK325
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK325

Quant Time: Feb 20 03:28:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 20 01:47:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	91077	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	84041	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	40314	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	22343	3.168	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.400%
7) Chloroethane-d5	1.536	69	19746	3.196	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	64.000%#
11) 1,1-Dichloroethene-d2	2.060	65	11144	3.276	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.600%
20) 2-Butanone-d5	3.831	46	30756	25.962	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	51.920%
24) Chloroform-d	4.252	84	42907	3.348	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	67.000%#
26) 1,2-Dichloroethane-d4	4.947	65	21666	3.617	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.400%
32) Benzene-d6	4.960	84	80125	3.178	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	63.600%#
36) 1,2-Dichloropropane-d6	5.992	67	22232	3.154	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	63.000%
41) Toluene-d8	7.243	98	74300	3.206	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	64.200%#
43) trans-1,3-Dichloroprop...	7.561	79	8484	3.188	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	63.800%
46) 2-Hexanone-d5	8.030	63	26833	28.243	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	56.480%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	13267	3.105	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	62.000%#
66) 1,2-Dichlorobenzene-d4	11.561	152	26126	3.563	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	71.200%#
Target Compounds						Qvalue
16) Methylene chloride	2.449	84	9790	1.604	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
Data File : VV034241.D
Acq On : 19 Feb 2024 14:16
Operator : SY/MD
Sample : VIBLK325
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK325

Quant Time: Feb 20 03:28:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 20 01:47:35 2024
Response via : Initial Calibration

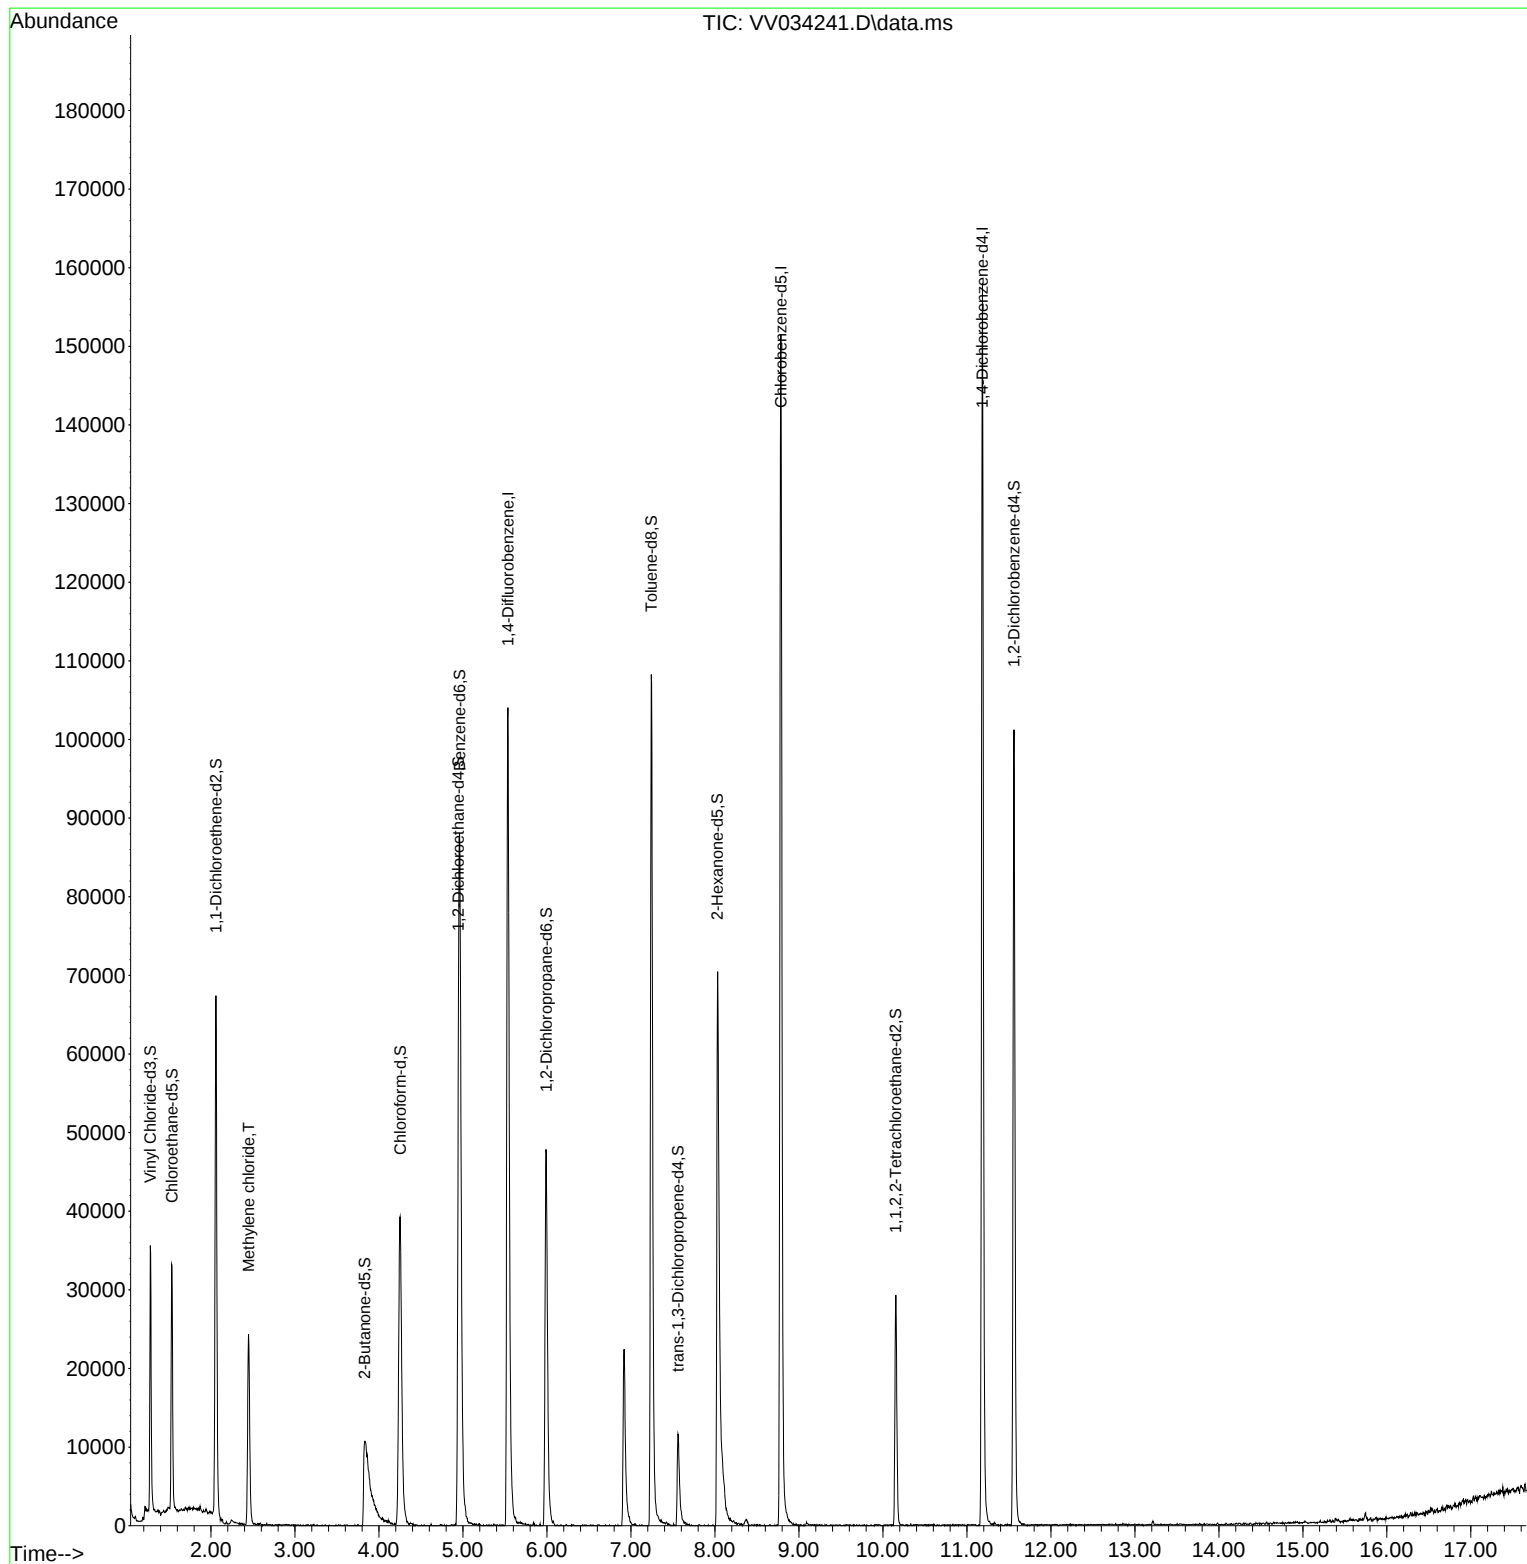

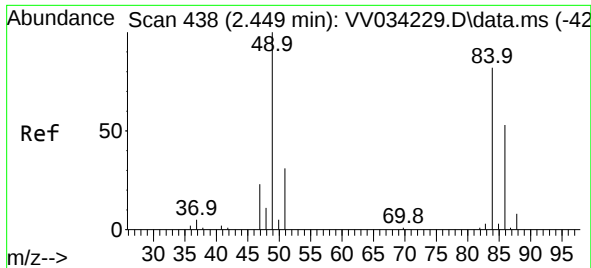

#16
Methylene chloride
Concen: 1.604 ug/L
RT: 2.449 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV034241.D
Acq: 19 Feb 2024 14:16

Instrument :
MSVOA_V
ClientSampleId :
VIBLK325

Tgt Ion: 84 Resp: 9790
Ion Ratio Lower Upper
84 100
86 65.0 44.7 83.1
49 128.0 93.7 173.9

