

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
 Data File : VV034233.D
 Acq On : 19 Feb 2024 11:01
 Operator : SY/MD
 Sample : P1513-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0U22

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	35598	39395	16.69%	2.020%
2	1.535	146	154	165	rBV	33137	38510	16.32%	1.974%
3	2.059	304	317	331	rBV	70392	103455	43.84%	5.304%
4	3.838	860	870	897	rBV2	11089	48306	20.47%	2.476%
5	4.252	984	999	1021	rBV2	39913	105015	44.50%	5.384%
6	4.956	1205	1218	1246	rBV3	93043	235999	100.00%	12.099%
7	5.535	1388	1398	1431	rBV	83700	173975	73.72%	8.919%
8	5.989	1528	1539	1565	rBV	50690	107650	45.61%	5.519%
9	6.918	1819	1828	1847	rBV2	24507	47843	20.27%	2.453%
10	7.243	1919	1929	1950	rBV	115506	206856	87.65%	10.605%
11	7.561	2020	2028	2052	rBV	12992	26798	11.36%	1.374%
12	8.034	2166	2175	2214	rBV	73530	170416	72.21%	8.736%
13	8.786	2399	2409	2437	rBV	124792	211311	89.54%	10.833%
14	9.487	2621	2627	2633	rBV5	1567	2446	1.04%	0.125%
15	9.873	2739	2747	2757	rBV5	1902	3045	1.29%	0.156%
16	10.152	2824	2834	2848	rBV2	30939	49885	21.14%	2.557%
17	10.484	2928	2937	2943	rBV4	1698	2428	1.03%	0.124%
18	10.863	3046	3055	3065	rVB3	1800	2684	1.14%	0.138%
19	11.185	3145	3155	3178	rBV	128243	205229	86.96%	10.521%
20	11.561	3262	3272	3292	rVB	106692	169376	71.77%	8.683%




Sum of corrected areas: 1950622

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
Data File : VV034233.D
Acq On : 19 Feb 2024 11:01
Operator : SY/MD
Sample : P1513-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0U22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

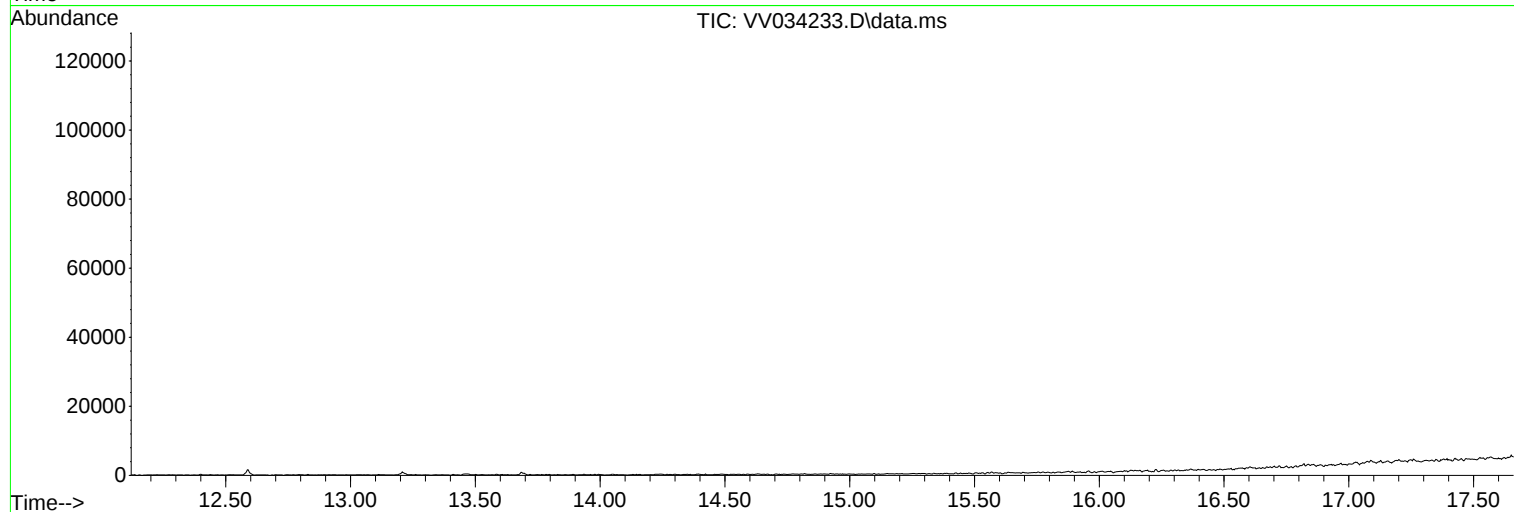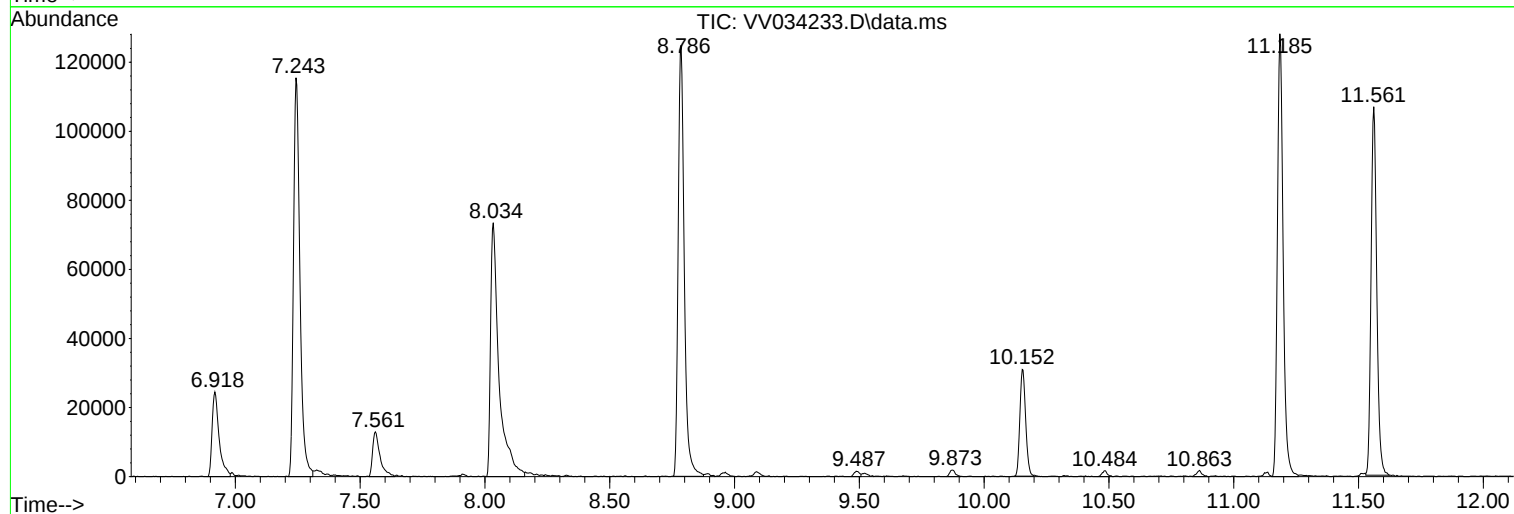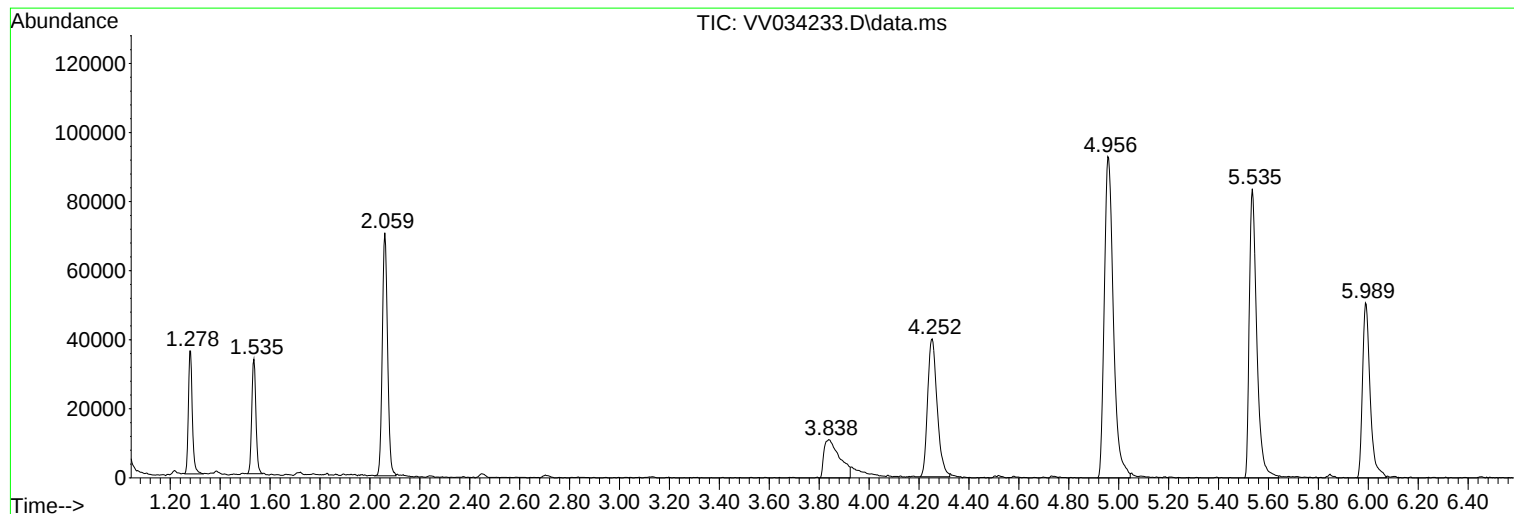

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
Data File : VV034233.D
Acq On : 19 Feb 2024 11:01
Operator : SY/MD
Sample : P1513-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0U22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
Data File : VV034233.D
Acq On : 19 Feb 2024 11:01
Operator : SY/MD
Sample : P1513-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0U22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc