

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
 Data File : VV034237.D
 Acq On : 19 Feb 2024 12:39
 Operator : SY/MD
 Sample : P1503-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNB2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	60	rBV3	1733	2027	1.21%	0.180%
2	1.282	67	75	85	rVB	17735	18598	11.13%	1.649%
3	1.388	101	108	116	rBV	12074	13417	8.03%	1.190%
4	1.462	117	131	137	rBV9	3968	7403	4.43%	0.656%
5	1.529	145	152	161	rVB	16458	18746	11.22%	1.662%
6	2.060	307	317	329	rBV	34474	49835	29.84%	4.419%
7	2.452	431	439	448	rBV2	2467	3981	2.38%	0.353%
8	3.793	849	856	887	rBV	21002	59811	35.81%	5.303%
9	4.252	983	999	1022	rBV	20069	52099	31.19%	4.619%
10	4.960	1206	1219	1248	rBV4	47314	122428	73.30%	10.855%
11	5.539	1389	1399	1418	rBV2	39856	81472	48.78%	7.224%
12	5.992	1529	1540	1558	rBV	26161	53474	32.01%	4.741%
13	6.921	1820	1829	1850	rBV2	12791	26147	15.65%	2.318%
14	7.246	1919	1930	1951	rBV	53719	97272	58.24%	8.624%
15	7.564	2021	2029	2049	rBV2	7920	15425	9.23%	1.368%
16	8.027	2164	2173	2209	rBV	80049	167030	100.00%	14.809%
17	8.786	2398	2409	2434	rBV	61343	104418	62.51%	9.258%
18	10.153	2825	2834	2848	rBV	26114	41242	24.69%	3.657%
19	11.188	3146	3156	3176	rBV	64388	100613	60.24%	8.921%
20	11.561	3262	3272	3292	rVB	57943	92421	55.33%	8.194%




Sum of corrected areas: 1127859

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
Data File : VV034237.D
Acq On : 19 Feb 2024 12:39
Operator : SY/MD
Sample : P1503-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

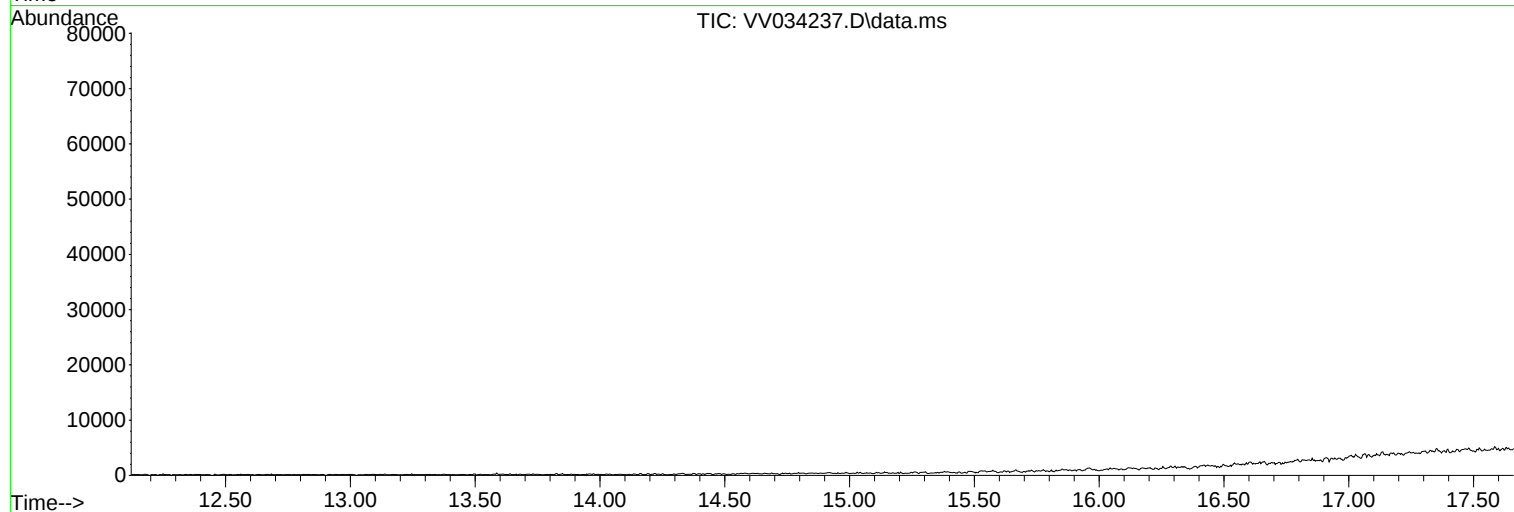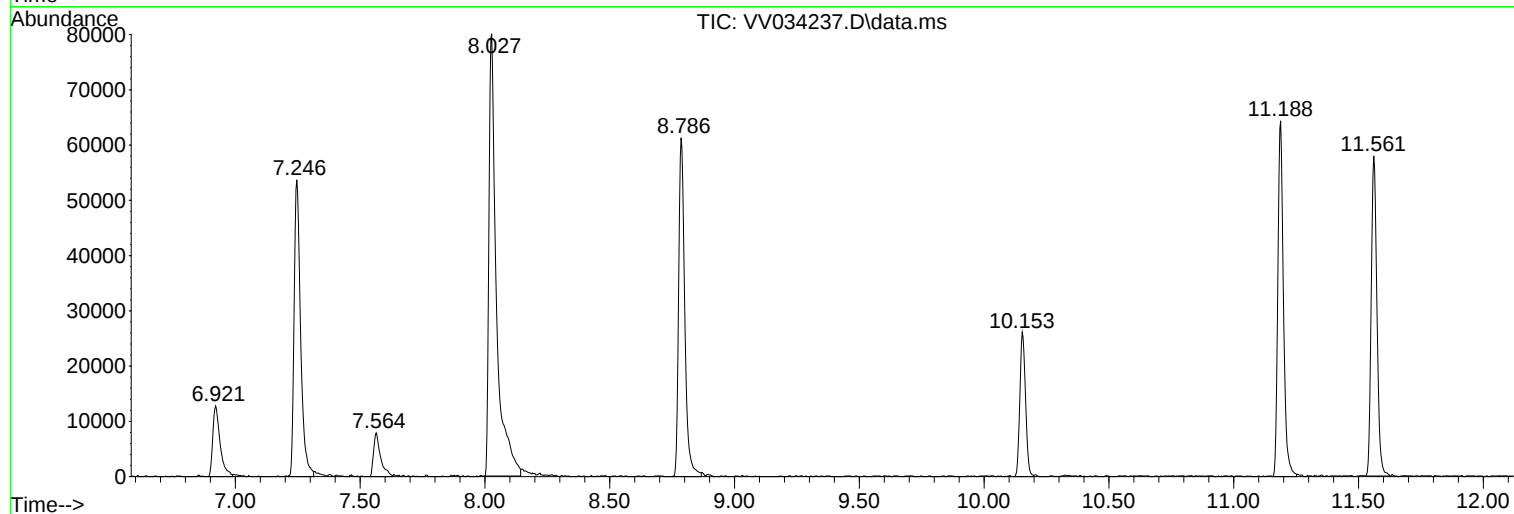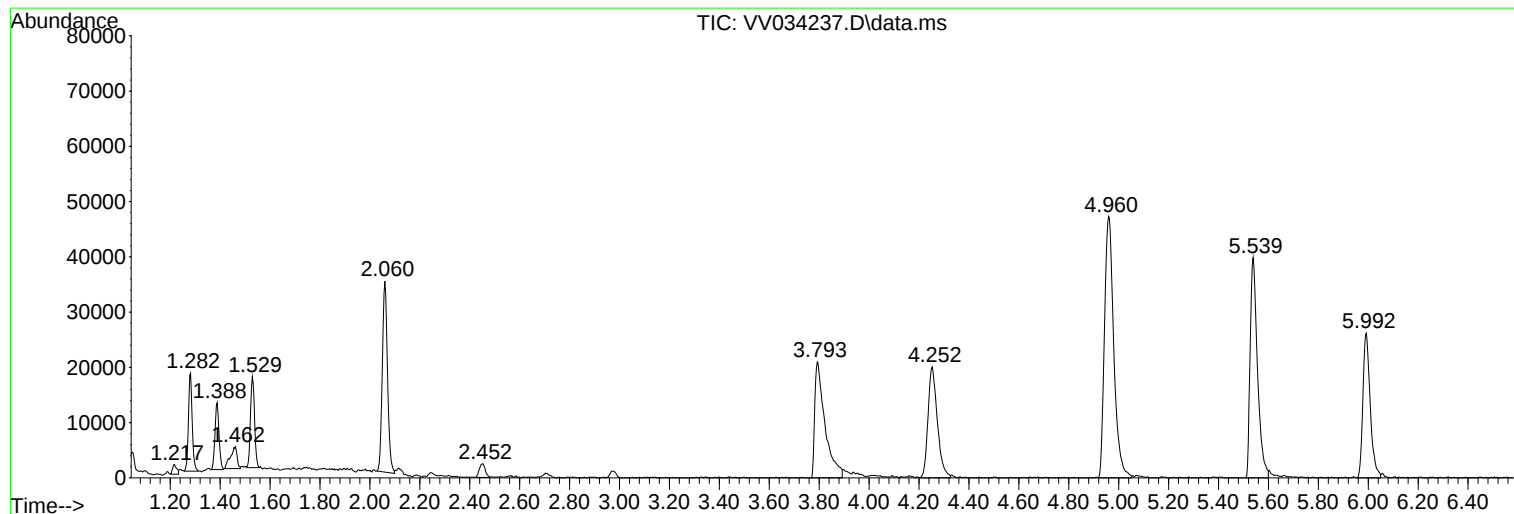

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
Data File : VV034237.D
Acq On : 19 Feb 2024 12:39
Operator : SY/MD
Sample : P1503-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
Data File : VV034237.D
Acq On : 19 Feb 2024 12:39
Operator : SY/MD
Sample : P1503-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------