


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021924\
Data File : VV034228.D
Acq On : 19 Feb 2024 08:20
Operator : SY/MD
Sample : BFB255
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB255

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Feb 22 00:18:57 2024

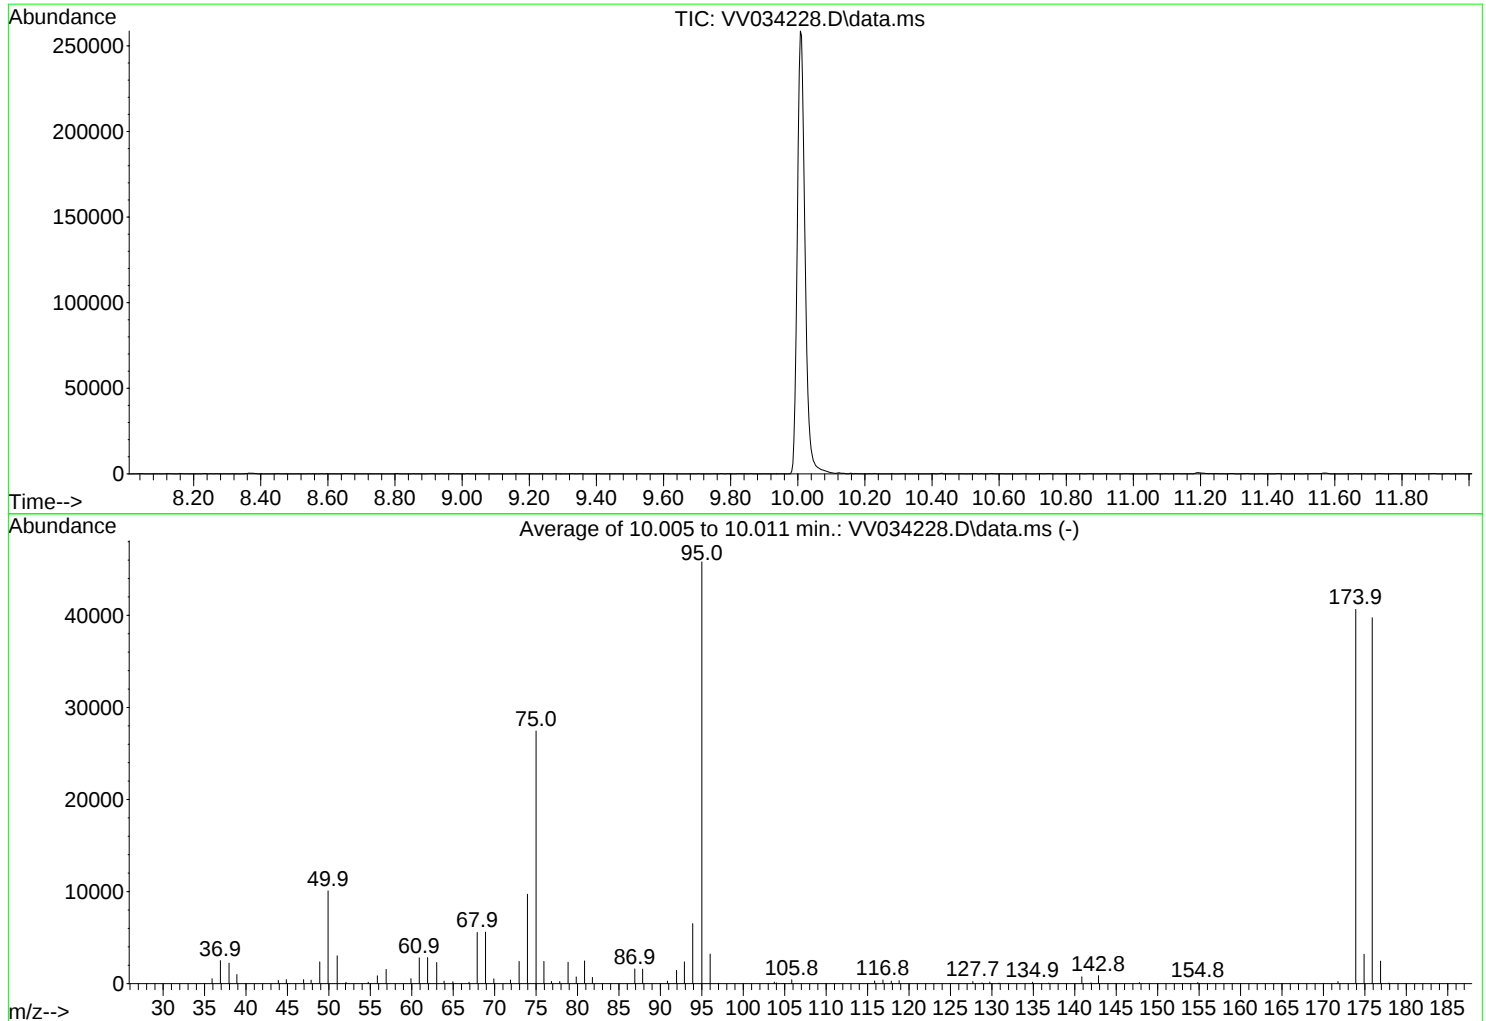

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	10076	PASS
75	95	30	80	59.9	27445	PASS
95	95	100	100	100.0	45811	PASS
96	95	5	9	7.0	3216	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.7	40656	PASS
175	174	5	9	7.9	3199	PASS
176	174	95	105	97.7	39739	PASS
177	176	5	10	6.2	2449	PASS

m/z	Abundance
74.80	119.0
94.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
35.90	530.0
36.90	2447.0
37.90	2096.0
38.90	963.0
43.90	314.0
44.90	374.0
46.90	459.0
47.90	353.0
48.90	2255.0
49.90	9777.0
51.00	2931.0
52.00	157.0
54.70	131.0
55.80	801.0
56.90	1398.0
59.90	602.0
60.90	2715.0
61.90	2797.0
63.00	2185.0
63.90	281.0
65.00	199.0
66.90	168.0
67.90	5365.0
68.90	5398.0
69.90	481.0
71.90	334.0
73.00	2303.0
74.00	9188.0
75.00	26160.0
75.90	2317.0
76.90	218.0
77.90	216.0
78.90	2111.0
79.80	645.0
80.90	2405.0
81.80	668.0
86.90	1569.0
87.90	1498.0
90.90	248.0
91.90	1398.0
92.90	2305.0
93.90	6122.0
95.00	43096.0
96.00	3243.0
103.70	277.0
104.80	101.0
105.80	357.0
115.80	262.0
116.90	375.0
117.80	291.0
118.80	325.0
127.70	208.0
129.80	156.0
134.90	163.0
140.90	741.0
141.90	130.0
142.90	862.0
147.80	108.0
154.80	137.0
171.80	210.0
173.90	37360.0
174.90	2981.0
175.90	36656.0
176.90	2286.0
177.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
35.90	555.0
36.90	2596.0
38.00	2308.0
38.90	1023.0
43.90	357.0
44.80	456.0
47.00	461.0
47.90	390.0
48.90	2450.0
49.90	10357.0
51.00	3126.0
52.10	176.0
54.80	157.0
55.90	874.0
56.90	1613.0
59.90	559.0
60.90	2888.0
61.90	2927.0
63.00	2407.0
63.90	301.0
65.00	229.0
66.90	167.0
67.90	5736.0
68.90	5735.0
69.90	559.0
71.90	409.0
73.00	2478.0
73.90	10024.0
75.00	28376.0
76.00	2488.0
76.80	252.0
77.80	234.0
78.90	2390.0
79.90	775.0
80.80	2571.0
81.80	724.0
86.90	1618.0
87.80	1627.0
90.80	299.0
92.00	1503.0
92.90	2426.0
93.90	6774.0
95.00	47320.0
96.00	3336.0
103.80	261.0
105.90	442.0
115.80	318.0
116.90	409.0
117.90	293.0
118.80	336.0
127.70	266.0
128.80	117.0
129.70	173.0
130.80	110.0
134.90	173.0
136.80	107.0
140.90	766.0
142.00	114.0
142.90	912.0
147.80	121.0
154.80	158.0
171.80	231.0
173.90	42208.0
174.90	3306.0
175.90	41192.0
176.90	2500.0
177.90	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
35.90	512.0
36.90	2467.0
38.00	2259.0
38.90	972.0
43.90	400.0
44.80	470.0
47.00	404.0
47.80	394.0
48.90	2364.0
49.90	10094.0
51.00	3033.0
52.10	137.0
54.80	200.0
55.90	898.0
56.90	1653.0
59.90	479.0
60.90	2806.0
61.90	2798.0
63.00	2303.0
63.90	264.0
64.90	209.0
66.90	149.0
67.90	5613.0
68.90	5657.0
69.90	548.0
71.90	439.0
72.90	2457.0
73.90	9917.0
75.00	27800.0
76.00	2419.0
76.90	253.0
77.80	240.0
78.80	2468.0
79.90	790.0
80.80	2422.0
81.80	638.0
86.90	1611.0
87.80	1602.0
90.80	312.0
92.00	1423.0
92.90	2343.0
93.90	6679.0
95.00	47016.0
96.00	3069.0
97.00	127.0
104.00	249.0
105.90	434.0
115.90	310.0
116.80	424.0
117.90	259.0
118.80	322.0
127.70	274.0
128.80	130.0
129.70	184.0
130.90	125.0
134.90	150.0
136.90	107.0
140.80	758.0
142.80	838.0
147.80	121.0
154.90	145.0
171.70	261.0
173.90	42400.0
174.90	3311.0
175.90	41368.0
176.90	2561.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255