


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022019\
Data File : VV009307.D
Acq On : 20 Feb 2019 18:07
Operator : SY/MD
Sample : BFB63
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB63

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM022019S.M
Title : VOC Analysis
Last Update : Thu Feb 21 03:53:15 2019

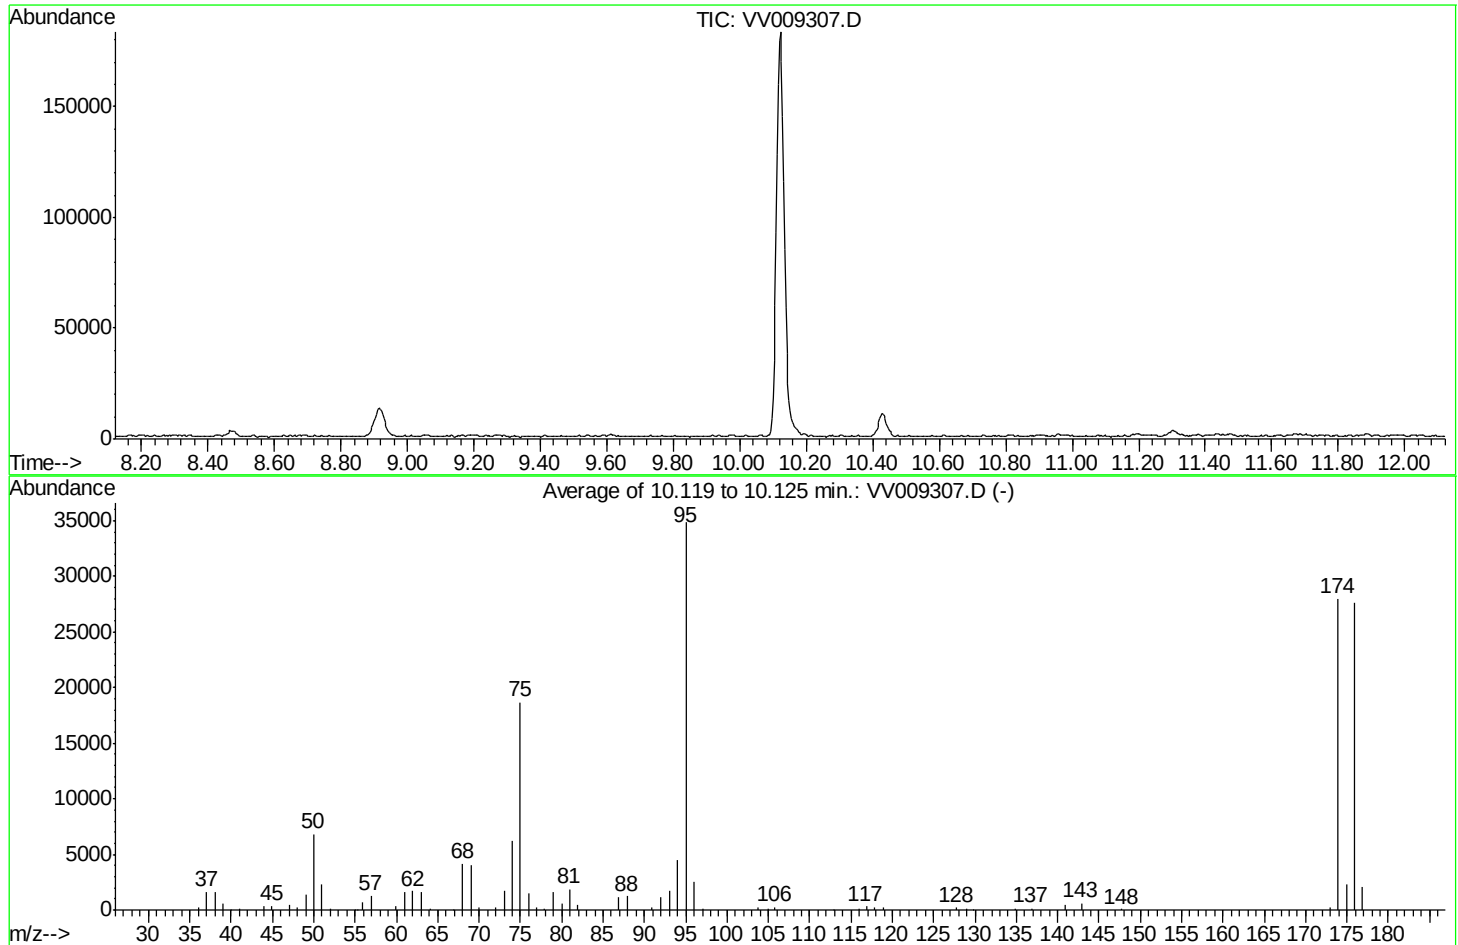

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	6838	PASS
75	95	30	80	53.5	18661	PASS
95	95	100	100	100.0	34853	PASS
96	95	5	9	7.2	2500	PASS
173	174	0.00	2	0.8	230	PASS
174	95	50	120	80.3	27981	PASS
175	174	5	9	8.4	2341	PASS
176	174	95	101	98.8	27658	PASS
177	176	5	9	7.3	2022	PASS

m/z	Abundance
38.90	172.0
40.00	116.0
41.10	141.0
42.90	194.0
43.90	325.0
55.00	121.0
56.90	105.0
66.80	152.0
69.90	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	279.0
37.00	1722.0
38.00	1640.0
39.00	749.0
39.90	172.0
40.90	211.0
43.00	175.0
44.00	610.0
45.00	406.0
47.00	484.0
48.00	269.0
49.00	1484.0
50.00	7214.0
51.00	2255.0
52.00	171.0
54.90	177.0
56.00	681.0
57.00	1414.0
59.90	362.0
61.00	1764.0
62.00	1839.0
63.00	1604.0
64.10	148.0
67.00	141.0
68.00	4402.0
69.00	4052.0
70.00	336.0
72.00	180.0
73.00	1763.0
74.00	6418.0
75.00	18928.0
76.00	1622.0
77.00	220.0
77.90	144.0
78.90	1602.0
80.00	615.0
80.90	1843.0
81.90	465.0
86.90	1346.0
87.90	1260.0
90.90	236.0
92.00	1170.0
93.00	1914.0
94.00	4834.0
95.00	34992.0
96.00	2648.0
97.10	108.0
103.80	219.0
105.00	112.0
105.80	247.0
115.90	167.0
116.90	327.0
117.80	184.0
118.90	230.0
127.80	184.0
128.90	131.0
134.90	106.0
136.80	146.0
140.90	487.0
142.90	546.0
147.70	105.0
173.90	27576.0
174.90	2304.0
175.90	27536.0
176.90	1946.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	236.0
37.00	1679.0
38.00	1657.0
39.00	770.0
39.90	161.0
40.90	213.0
43.00	192.0
43.90	637.0
45.00	393.0
47.00	454.0
48.00	244.0
49.00	1497.0
50.00	7055.0
51.00	2404.0
52.00	134.0
54.90	175.0
56.00	698.0
57.00	1496.0
60.00	409.0
61.00	1703.0
62.00	1753.0
63.00	1682.0
64.10	154.0
67.00	150.0
68.00	4306.0
69.00	4113.0
70.00	350.0
72.00	206.0
73.00	1751.0
74.00	6472.0
75.00	19352.0
76.00	1506.0
76.90	228.0
77.90	114.0
78.90	1685.0
80.00	644.0
80.90	1899.0
81.90	429.0
86.90	1211.0
87.90	1283.0
90.90	220.0
92.00	1233.0
93.00	1722.0
94.00	4672.0
95.00	36104.0
96.00	2590.0
97.10	128.0
103.80	232.0
105.00	131.0
105.80	230.0
115.90	142.0
116.90	309.0
117.80	211.0
118.80	236.0
127.70	196.0
128.90	108.0
134.90	107.0
136.80	144.0
140.90	558.0
142.90	597.0
147.70	111.0
172.90	356.0
173.90	28704.0
174.90	2446.0
175.90	28592.0
176.90	2109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	239.0
37.00	1550.0
38.00	1547.0
39.00	737.0
39.90	125.0
40.90	197.0
43.10	198.0
43.90	665.0
44.90	340.0
47.00	372.0
48.00	213.0
49.00	1349.0
50.00	6247.0
51.00	2243.0
54.80	143.0
55.20	149.0
55.90	709.0
57.00	1354.0
60.00	377.0
61.00	1492.0
62.00	1564.0
63.00	1479.0
64.00	150.0
67.00	180.0
68.00	3811.0
69.00	3801.0
70.00	335.0
72.00	193.0
73.00	1659.0
74.00	5930.0
75.00	17704.0
76.00	1311.0
76.90	234.0
78.90	1668.0
80.00	549.0
80.90	1833.0
81.90	365.0
86.90	1045.0
87.90	1203.0
90.90	186.0
92.00	1142.0
93.00	1503.0
94.00	4114.0
95.00	33464.0
96.00	2263.0
97.10	134.0
103.80	213.0
104.90	140.0
105.80	224.0
112.90	105.0
115.90	111.0
116.90	276.0
117.80	213.0
118.80	223.0
127.70	179.0
129.70	108.0
136.80	127.0
140.80	517.0
142.90	616.0
147.80	102.0
172.90	334.0
173.90	27664.0
174.90	2273.0
175.90	26848.0
176.90	2012.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63