

Data File : VV014627.D
Acq On : 20 Feb 2020 16:36
Operator : SY/MD
Sample : L1607-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN6

Quant Time: Feb 21 03:35:22 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 21 03:31:59 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	273417	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	255584	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	123811	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	34543	32.90	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	65.80%
7) Chloroethane-d5	1.59	69	29579	40.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.10%
11) 1,1-Dichloroethene-d2	2.13	63	53453	30.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.02%
21) 2-Butanone-d5	3.94	46	84567	97.12	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.12%
24) Chloroform-d	4.40	84	132433	43.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.50%
26) 1,2-Dichloroethane-d4	5.08	65	90873	47.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.68%
32) Benzene-d6	5.10	84	273061	44.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.34%
36) 1,2-Dichloropropane-d6	6.12	67	84093	45.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.36%
41) Toluene-d8	7.36	98	255883	43.51	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.02%
43) trans-1,3-Dichloropropene-	7.66	79	44159	43.50	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.00%
47) 2-Hexanone-d5	8.13	63	70699	96.10	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.10%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	120323	48.15	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.30%
64) 1,2-Dichlorobenzene-d4	11.67	152	103928	47.51	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.02%

Target Compounds

					Qvalue	
10) 1,1,2-Trichloro-1,2,2-trif	2.13	101	691	0.766	ug/L #	17
13) Acetone	2.20	43	1773	2.373	ug/L	91
25) Chloroform	4.42	83	9323	2.905	ug/L	87
34) Trichloroethene	5.96	95	45730	25.254	ug/L	97
39) cis-1,3-Dichloropropene	7.03	75	2613	0.893	ug/L #	31
48) 2-Hexanone	8.13	43	7942	4.977	ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data File : VV014627.D

```
Acq On       : 20 Feb 2020   16:36
Operator    : SY/MD
Sample      : L1607-03
Misc       : 5.0mL/MSVOA_V/WATER
ALS Vial    : 11      Sample Multiplier: 1
```

Instrument :
MSVOA_V
ClientSampleId :
C0AN6

Quant Time: Feb 21 03:35:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 21 03:31:59 2020
Response via : Initial Calibration

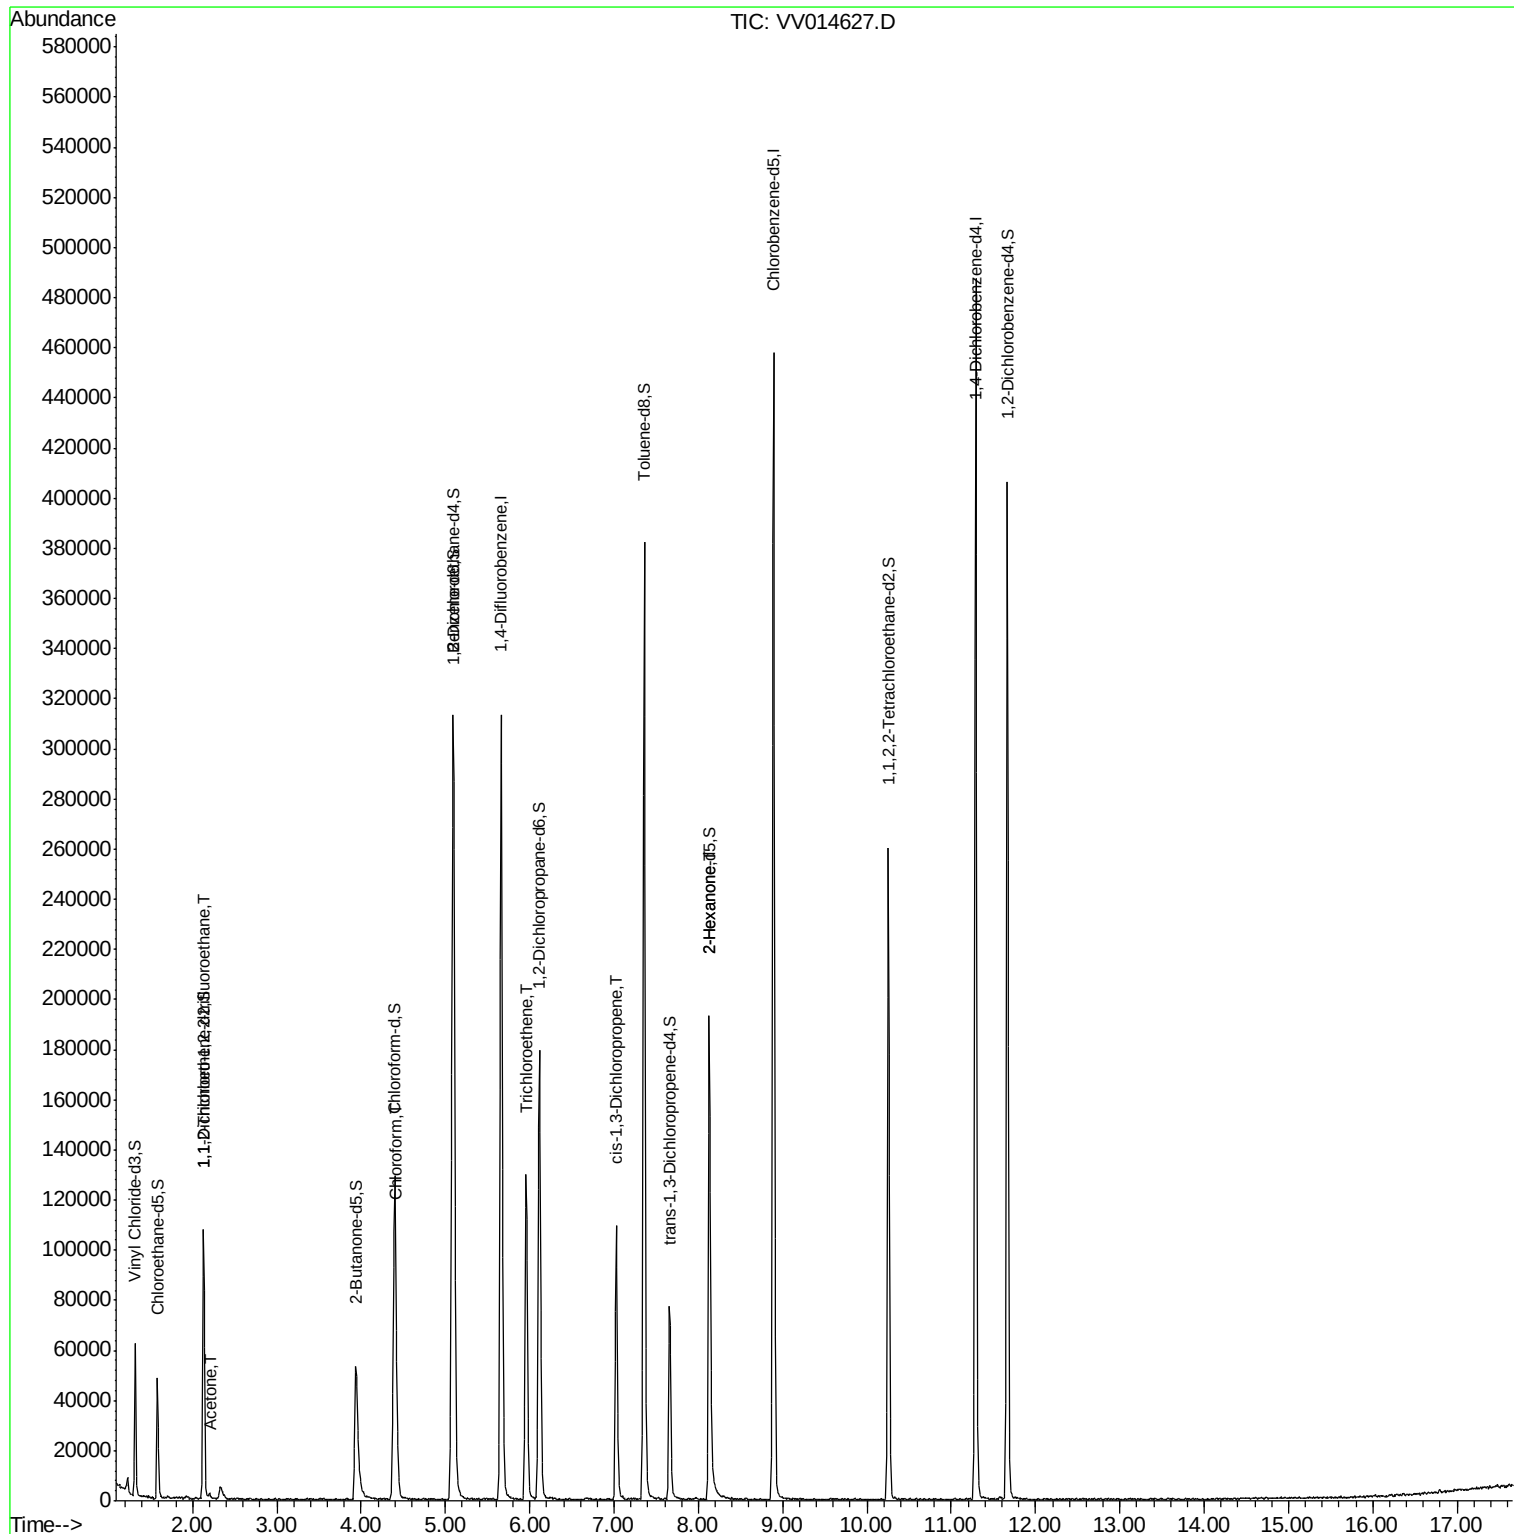

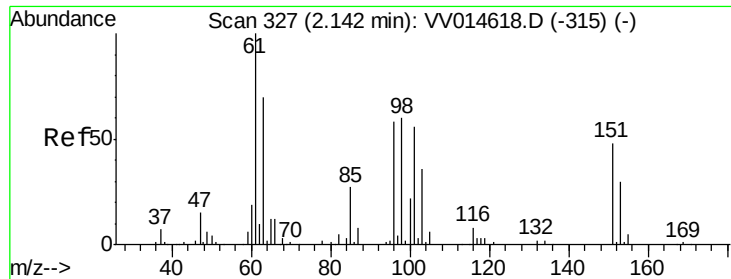

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.766 ug/L

RT: 2.13 min Scan# 323

Delta R.T. -0.01 min

Lab File: VV014627.D

Acq: 20 Feb 2020 16:36

Instrument :

MSVOA_V

ClientSampled :

COAN6


Tgt Ion: 101 Resp: 691

Ion Ratio Lower Upper

101 100

85 0.0 35.4 53.0#




151 0.0 65.4 98.2#

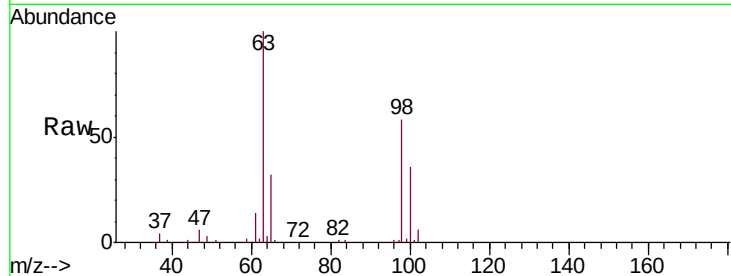

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VV0

Ion 151.00 (150.70 to 151.70): V

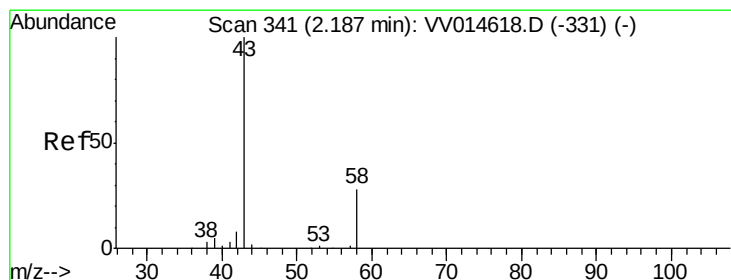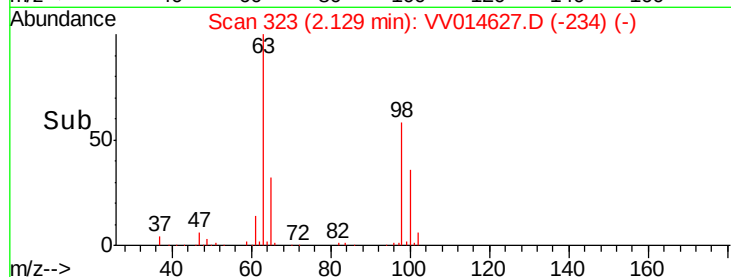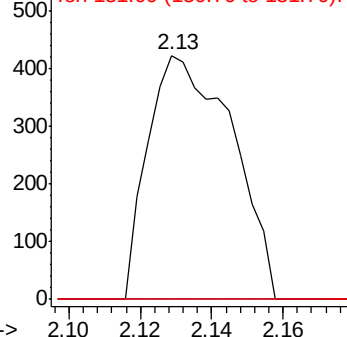

#13

Acetone

Concen: 2.373 ug/L

RT: 2.20 min Scan# 345

Delta R.T. 0.01 min

Lab File: VV014627.D


Acq: 20 Feb 2020 16:36

Tgt Ion: 43 Resp: 1773

Ion Ratio Lower Upper



43 100


58 34.0 0.0 58.8

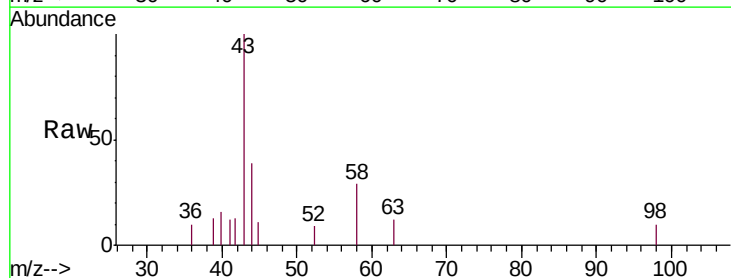

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 58.00 (57.70 to 58.70): VV0



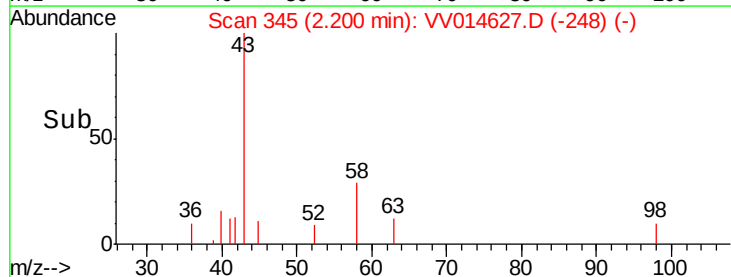
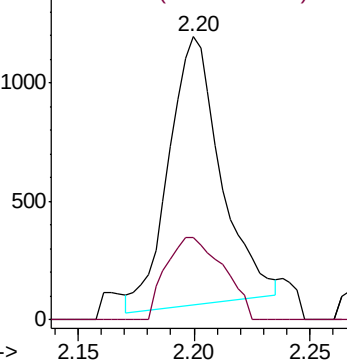


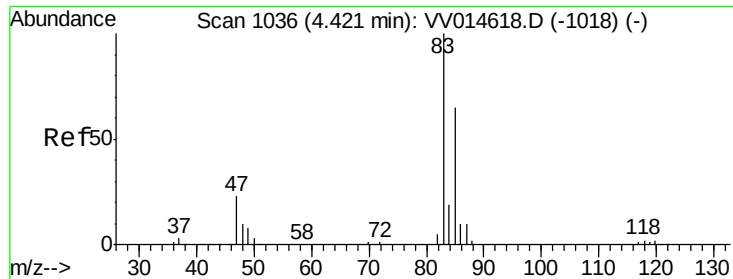

#25
Chloroform
Concen: 2.905 ug/L
RT: 4.42 min Scan# 1036
Delta R.T. -0.00 min
Lab File: VV014627.D
Acq: 20 Feb 2020 16:36




Instrument :
MSVOA_V
ClientSampled :
COAN6


Tgt Ion: 83 Resp: 9323
Ion Ratio Lower Upper
83 100
85 74.5 45.0 83.6

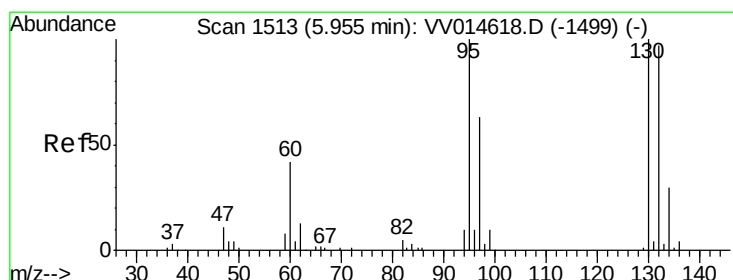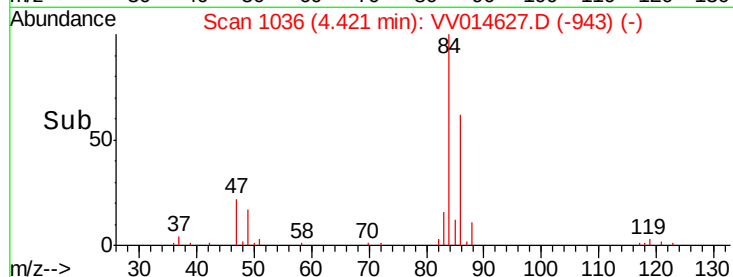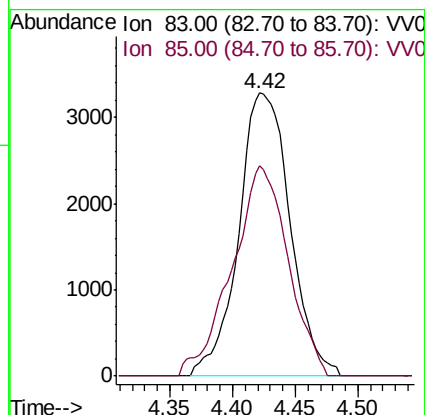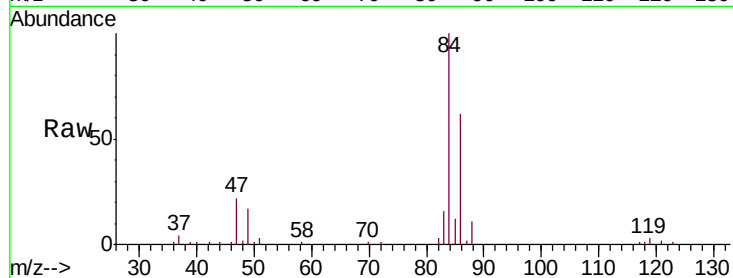

#34
Trichloroethene
Concen: 25.254 ug/L
RT: 5.96 min Scan# 1514
Delta R.T. 0.00 min
Lab File: VV014627.D
Acq: 20 Feb 2020 16:36

Tgt Ion: 95 Resp: 45730
Ion Ratio Lower Upper
95 100
97 65.7 45.3 84.1
132 96.8 69.6 129.2
130 101.3 74.0 137.4


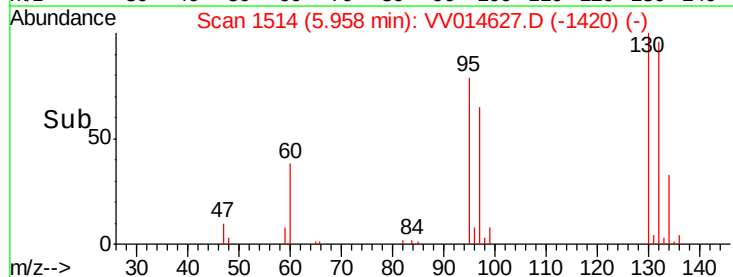
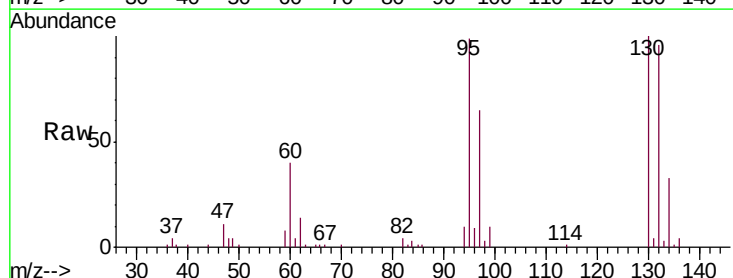
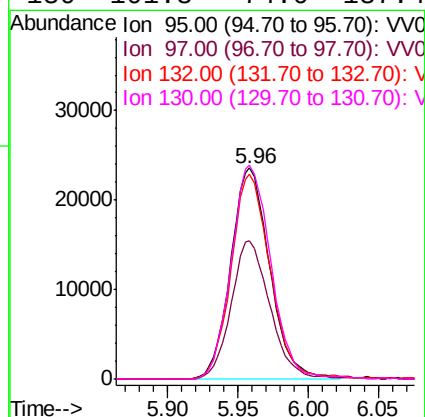


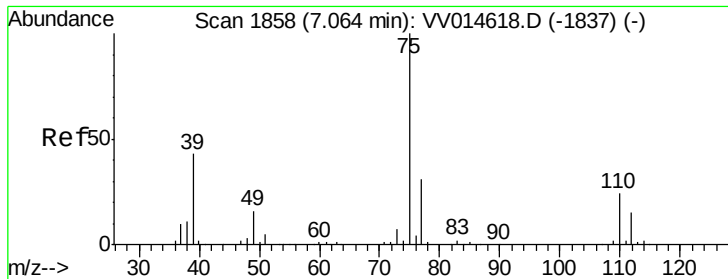

#39
 cis-1,3-Dichloropropene
 Concen: 0.893 ug/L
 RT: 7.03 min Scan# 1846
 Delta R.T. -0.04 min
 Lab File: VV014627.D
 Acq: 20 Feb 2020 16:36

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN6

Tgt Ion: 75 Resp: 2613
 Ion Ratio Lower Upper
 75 100
 77 68.9 21.7 40.3#

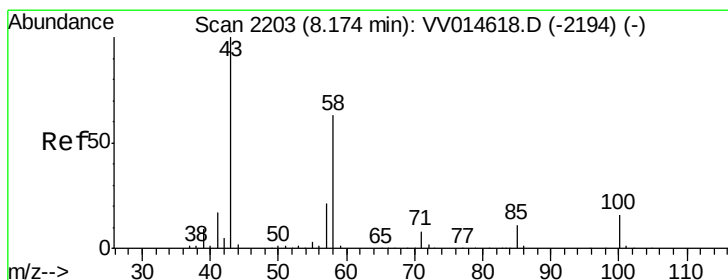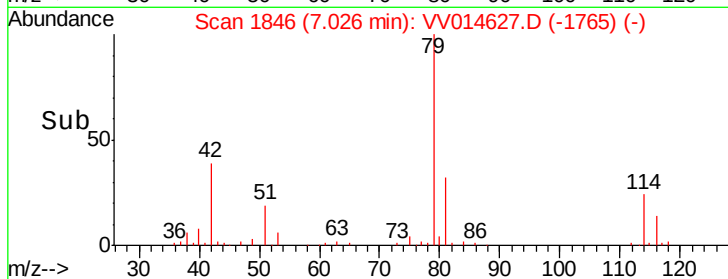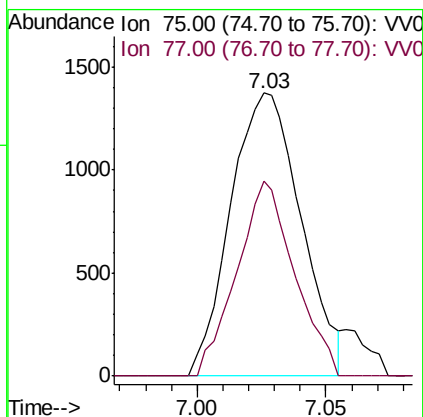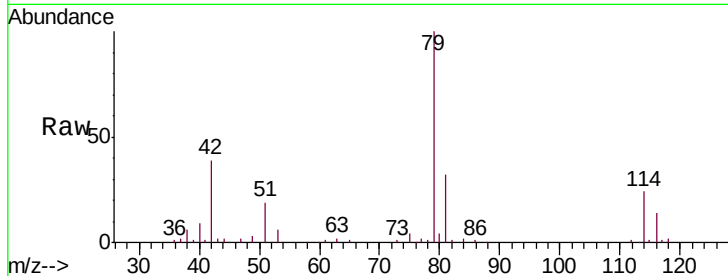

#48
 2-Hexanone
 Concen: 4.977 ug/L
 RT: 8.13 min Scan# 2189
 Delta R.T. -0.05 min
 Lab File: VV014627.D
 Acq: 20 Feb 2020 16:36

Tgt Ion: 43 Resp: 7942
 Ion Ratio Lower Upper
 43 100
 58 32.5 50.4 75.6#
 57 27.9 17.8 26.6#
 100 0.9 12.6 19.0#

