

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014621.D
 Acq On : 20 Feb 2020 14:16
 Operator : SY/MD
 Sample : L1584-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.132	316	324	336	rVB	115971	161707	19.09%	2.708%
2	2.624	474	477	479	rBV2	503	302	0.04%	0.005%
3	2.807	533	534	536	rBV	372	117	0.01%	0.002%
4	2.849	545	547	549	rBV	250	122	0.01%	0.002%
5	2.862	549	551	552	rBV	471	230	0.03%	0.004%
6	2.897	559	562	563	rBV	224	121	0.01%	0.002%
7	2.987	587	590	592	rBV2	362	182	0.02%	0.003%
8	3.061	611	613	615	rVB	568	155	0.02%	0.003%
9	3.074	615	617	620	rBV2	441	260	0.03%	0.004%
10	3.151	639	641	645	rVB2	454	195	0.02%	0.003%
11	3.174	645	648	649	rBV	265	118	0.01%	0.002%
12	3.334	695	698	703	rVB2	436	373	0.04%	0.006%
13	3.425	723	726	727	rBV2	181	111	0.01%	0.002%
14	3.431	727	728	731	rVV3	393	178	0.02%	0.003%
15	3.460	735	737	739	rBV	394	165	0.02%	0.003%
16	3.605	780	782	786	rVB2	309	178	0.02%	0.003%
17	3.643	790	794	797	rBV2	278	239	0.03%	0.004%
18	3.720	813	818	820	rBV2	305	208	0.02%	0.003%
19	3.769	831	833	837	rVB2	225	160	0.02%	0.003%
20	3.788	837	839	841	rBV	252	111	0.01%	0.002%
21	3.826	850	851	853	rBV	367	132	0.02%	0.002%
22	3.923	871	881	905	rBV	57774	151204	17.85%	2.532%
23	4.646	1104	1106	1108	rBV	481	274	0.03%	0.005%
24	4.820	1158	1160	1162	rBV2	287	100	0.01%	0.002%
25	4.900	1183	1185	1190	rBV2	220	170	0.02%	0.003%
26	4.955	1200	1202	1208	rVB	229	167	0.02%	0.003%
27	4.981	1208	1210	1211	rBV2	241	91	0.01%	0.002%
28	5.093	1229	1245	1270	rBV2	334037	847028	100.00%	14.183%
29	5.482	1364	1366	1371	rBV	497	224	0.03%	0.004%
30	5.559	1388	1390	1392	rBV	420	249	0.03%	0.004%
31	5.662	1409	1422	1451	rBV	278598	545720	64.43%	9.138%
32	5.949	1504	1511	1517	rBV7	1927	3076	0.36%	0.052%
33	6.113	1549	1562	1590	rBV	192278	390915	46.15%	6.546%
34	6.495	1677	1681	1683	rBV	416	289	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014621.D
 Acq On : 20 Feb 2020 14:16
 Operator : SY/MD
 Sample : L1584-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

35	6.508	1683	1685	1687	rBV	484	214	0.03%	0.004%
36	6.547	1695	1697	1698	rBV	194	85	0.01%	0.001%
37	6.556	1698	1700	1702	rVB	321	128	0.02%	0.002%
38	6.572	1702	1705	1709	rBV3	505	450	0.05%	0.008%
39	6.743	1756	1758	1759	rBV	208	78	0.01%	0.001%
40	6.765	1762	1765	1768	rBV2	664	340	0.04%	0.006%
41	6.846	1785	1790	1793	rBV2	596	426	0.05%	0.007%
42	6.910	1806	1810	1812	rBV	337	188	0.02%	0.003%
43	6.968	1827	1828	1829	rBV	210	42	0.00%	0.001%
44	7.026	1836	1846	1868	rBV	114049	201995	23.85%	3.382%
45	7.357	1934	1949	1966	rBV	410610	716983	84.65%	12.006%
46	7.659	2034	2043	2060	rBV	84377	141412	16.70%	2.368%
47	7.871	2104	2109	2115	rBV3	742	917	0.11%	0.015%
48	8.125	2178	2188	2217	rBV	176194	361484	42.68%	6.053%
49	8.405	2271	2275	2276	rBV3	612	393	0.05%	0.007%
50	8.537	2314	2316	2319	rVB2	629	310	0.04%	0.005%
51	8.653	2350	2352	2355	rBV2	433	321	0.04%	0.005%
52	8.685	2361	2362	2364	rBV	258	136	0.02%	0.002%
53	8.743	2378	2380	2381	rBV	252	85	0.01%	0.001%
54	8.891	2415	2426	2449	rBV	396566	649178	76.64%	10.870%
55	9.202	2522	2523	2525	rBV	377	190	0.02%	0.003%
56	9.247	2535	2537	2538	rBV2	333	127	0.01%	0.002%
57	9.286	2545	2549	2552	rVB2	352	217	0.03%	0.004%
58	9.411	2586	2588	2589	rBV2	267	88	0.01%	0.001%
59	9.546	2628	2630	2634	rBV3	435	273	0.03%	0.005%
60	9.723	2684	2685	2689	rBV2	410	278	0.03%	0.005%
61	9.871	2729	2731	2734	rBV	302	118	0.01%	0.002%
62	9.907	2739	2742	2745	rBV3	335	309	0.04%	0.005%
63	9.942	2750	2753	2754	rBV	343	141	0.02%	0.002%
64	10.038	2781	2783	2786	rBV	344	257	0.03%	0.004%
65	10.254	2830	2850	2866	rBV	270595	430519	50.83%	7.209%
66	10.347	2877	2879	2881	rBV	499	183	0.02%	0.003%
67	10.389	2889	2892	2894	rBV2	387	233	0.03%	0.004%
68	10.492	2922	2924	2926	rBV	379	86	0.01%	0.001%
69	10.720	2992	2995	2997	rBV2	179	104	0.01%	0.002%
70	10.842	3029	3033	3036	rVB2	442	246	0.03%	0.004%
71	10.862	3036	3039	3043	rBV2	267	242	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014621.D
Acq On : 20 Feb 2020 14:16
Operator : SY/MD
Sample : L1584-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM5

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Title : VOC Analysis

72	11.289	3158	3172	3192	rBV	420834	661002	78.04%	11.068%
73	11.534	3244	3248	3250	rBV3	489	362	0.04%	0.006%
74	11.579	3254	3262	3272	rBV8	2896	5356	0.63%	0.090%
75	11.665	3277	3289	3308	rBV	434334	690740	81.55%	11.566%
76	12.521	3554	3555	3556	rBV	169	56	0.01%	0.001%
77	12.787	3636	3638	3641	rBV	375	140	0.02%	0.002%
78	13.222	3770	3773	3775	rBV	239	127	0.01%	0.002%
79	13.623	3895	3898	3901	rBV	337	241	0.03%	0.004%
80	13.855	3968	3970	3972	rBV2	360	154	0.02%	0.003%
81	14.218	4082	4083	4084	rBV	411	136	0.02%	0.002%


Sum of corrected areas: 5971961

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014621.D
Acq On : 20 Feb 2020 14:16
Operator : SY/MD
Sample : L1584-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

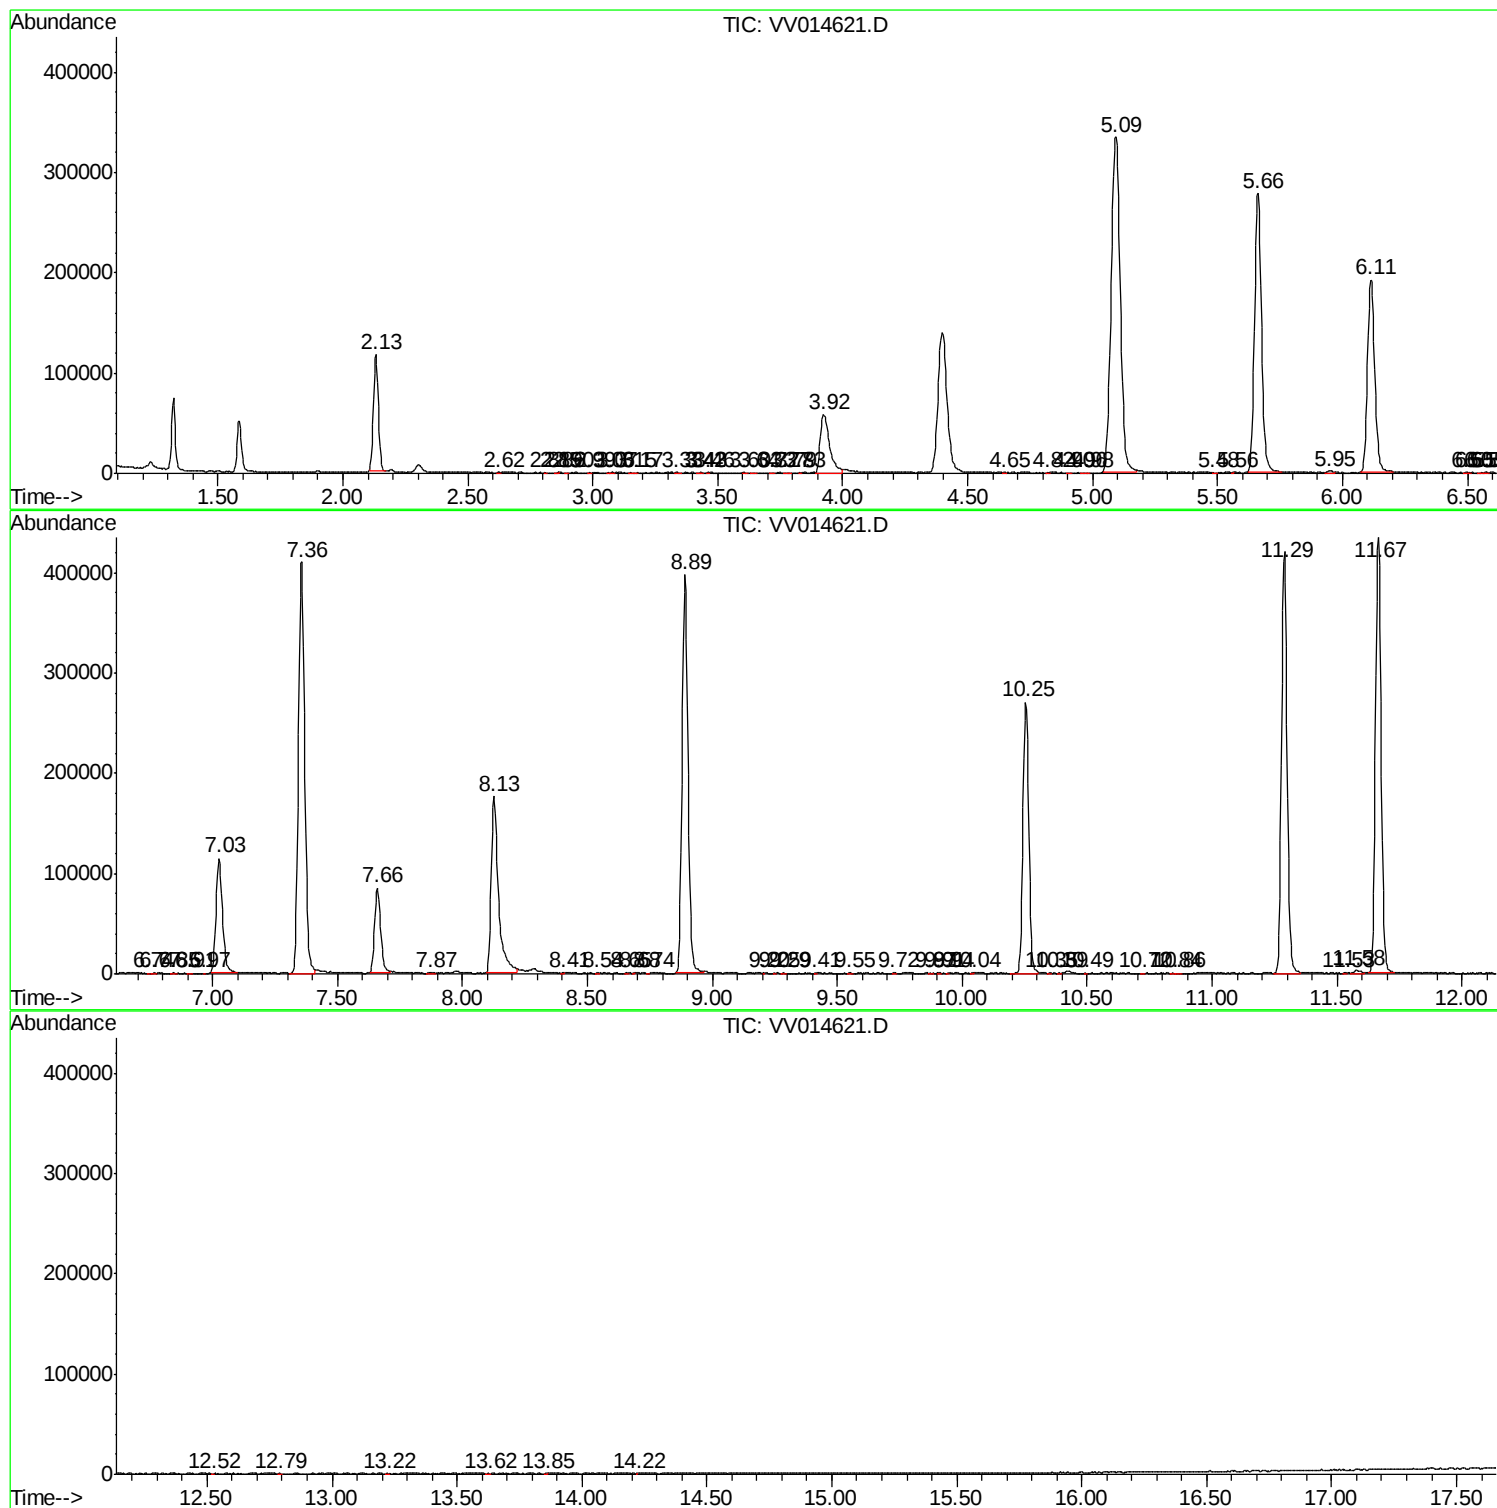

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014621.D
Acq On : 20 Feb 2020 14:16
Operator : SY/MD
Sample : L1584-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014621.D
Acq On : 20 Feb 2020 14:16
Operator : SY/MD
Sample : L1584-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc