

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014623.D
 Acq On : 20 Feb 2020 15:03
 Operator : SY/MD
 Sample : L1584-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.495	434	437	438	rBV2	329	186	0.02%	0.003%
2	2.769	520	522	526	rBV2	365	238	0.03%	0.004%
3	2.811	532	535	538	rVB3	388	259	0.03%	0.004%
4	2.920	568	569	574	rBV2	376	213	0.03%	0.004%
5	2.975	584	586	589	rVB2	246	106	0.01%	0.002%
6	3.042	605	607	608	rBV2	384	153	0.02%	0.003%
7	3.116	628	630	633	rVB2	376	139	0.02%	0.002%
8	3.306	686	689	691	rBV	377	175	0.02%	0.003%
9	3.348	701	702	705	rBV	173	85	0.01%	0.001%
10	3.373	705	710	718	rVB4	448	574	0.07%	0.009%
11	3.438	729	730	731	rVB4	115	22	0.00%	0.000%
12	3.450	732	734	736	rBV2	393	136	0.02%	0.002%
13	3.466	737	739	741	rBV2	236	75	0.01%	0.001%
14	3.502	748	750	753	rVB2	545	248	0.03%	0.004%
15	3.528	753	758	762	rBV2	253	247	0.03%	0.004%
16	3.740	822	824	828	rVB3	505	190	0.02%	0.003%
17	3.836	851	854	855	rBV	299	91	0.01%	0.002%
18	3.852	855	859	861	rBV3	501	289	0.03%	0.005%
19	3.923	869	881	906	rBV2	58136	150144	18.11%	2.479%
20	4.688	1116	1119	1121	rBV2	751	451	0.05%	0.007%
21	4.955	1200	1202	1204	rBV3	486	191	0.02%	0.003%
22	4.994	1212	1214	1217	rBV	339	181	0.02%	0.003%
23	5.093	1227	1245	1268	rBV2	325303	829104	100.00%	13.688%
24	5.460	1357	1359	1363	rVB5	566	303	0.04%	0.005%
25	5.515	1372	1376	1377	rBV2	817	412	0.05%	0.007%
26	5.560	1389	1390	1392	rVB2	480	113	0.01%	0.002%
27	5.576	1392	1395	1396	rBV	245	116	0.01%	0.002%
28	5.659	1409	1421	1448	rBV	316341	631346	76.15%	10.423%
29	6.113	1548	1562	1588	rBV	185383	380857	45.94%	6.288%
30	6.344	1632	1634	1635	rBV2	437	195	0.02%	0.003%
31	6.547	1695	1697	1700	rBV2	379	172	0.02%	0.003%
32	6.598	1712	1713	1715	rBV2	444	159	0.02%	0.003%
33	6.794	1771	1774	1775	rVB	346	147	0.02%	0.002%
34	6.807	1775	1778	1779	rBV	325	186	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014623.D
 Acq On : 20 Feb 2020 15:03
 Operator : SY/MD
 Sample : L1584-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

35	6.913	1808	1811	1814	rBV2	172	83	0.01%	0.001%
36	6.939	1814	1819	1822	rBV3	599	436	0.05%	0.007%
37	6.968	1825	1828	1830	rBV2	159	114	0.01%	0.002%
38	6.981	1830	1832	1835	rBV2	581	359	0.04%	0.006%
39	7.026	1835	1846	1865	rBV	112477	199450	24.06%	3.293%
40	7.267	1919	1921	1923	rBV	389	149	0.02%	0.002%
41	7.357	1935	1949	1972	rBV	396519	702417	84.72%	11.597%
42	7.659	2033	2043	2058	rBV2	82760	139709	16.85%	2.307%
43	8.042	2160	2162	2163	rBV	333	129	0.02%	0.002%
44	8.125	2178	2188	2218	rBV	181606	361504	43.60%	5.968%
45	8.463	2291	2293	2295	rBV3	360	165	0.02%	0.003%
46	8.505	2305	2306	2309	rBV	290	116	0.01%	0.002%
47	8.524	2309	2312	2313	rBV	448	265	0.03%	0.004%
48	8.585	2329	2331	2333	rBV	352	136	0.02%	0.002%
49	8.605	2335	2337	2342	rVB2	490	266	0.03%	0.004%
50	8.637	2342	2347	2348	rBV3	414	284	0.03%	0.005%
51	8.891	2414	2426	2448	rBV	472143	766785	92.48%	12.659%
52	9.087	2482	2487	2493	rBV3	749	734	0.09%	0.012%
53	9.238	2533	2534	2535	rBV3	223	70	0.01%	0.001%
54	9.270	2541	2544	2547	rBV	447	267	0.03%	0.004%
55	9.305	2550	2555	2558	rBV2	465	470	0.06%	0.008%
56	9.331	2561	2563	2565	rBV2	495	211	0.03%	0.003%
57	9.367	2572	2574	2576	rBV	404	229	0.03%	0.004%
58	9.441	2592	2597	2600	rBV3	470	431	0.05%	0.007%
59	9.486	2610	2611	2613	rBV	242	89	0.01%	0.001%
60	9.624	2652	2654	2657	rBV2	558	356	0.04%	0.006%
61	9.836	2716	2720	2726	rVB3	438	437	0.05%	0.007%
62	9.871	2728	2731	2732	rBV2	462	300	0.04%	0.005%
63	10.064	2785	2791	2794	rBV4	941	1035	0.12%	0.017%
64	10.154	2817	2819	2820	rBV	392	97	0.01%	0.002%
65	10.254	2838	2850	2872	rBV	269824	421550	50.84%	6.960%
66	10.408	2893	2898	2900	rBV4	1249	909	0.11%	0.015%
67	10.559	2943	2945	2947	rBV	590	287	0.03%	0.005%
68	10.595	2955	2956	2959	rVB	528	192	0.02%	0.003%
69	10.685	2982	2984	2985	rBV	325	80	0.01%	0.001%
70	10.714	2991	2993	2997	rVB	614	264	0.03%	0.004%
71	10.746	3001	3003	3005	rBV	415	231	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014623.D
 Acq On : 20 Feb 2020 15:03
 Operator : SY/MD
 Sample : L1584-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

72	10.756	3005	3006	3008	rVB	637	128	0.02%	0.002%
73	10.788	3015	3016	3020	rBV2	349	220	0.03%	0.004%
74	10.913	3053	3055	3056	rBV	231	75	0.01%	0.001%
75	10.952	3064	3067	3069	rBV3	575	359	0.04%	0.006%
76	11.289	3160	3172	3190	rBV	497147	772843	93.21%	12.759%
77	11.495	3232	3236	3238	rBV	465	348	0.04%	0.006%
78	11.575	3253	3261	3269	rBV7	3503	6705	0.81%	0.111%
79	11.666	3278	3289	3305	rBV	430022	675891	81.52%	11.159%
80	11.945	3374	3376	3377	rBV	134	34	0.00%	0.001%
81	11.961	3378	3381	3386	rVV3	578	505	0.06%	0.008%
82	12.000	3390	3393	3394	rBV	210	94	0.01%	0.002%
83	12.016	3394	3398	3401	rBV2	513	424	0.05%	0.007%
84	12.174	3441	3447	3449	rBV3	506	524	0.06%	0.009%
85	12.881	3665	3667	3669	rBV	450	185	0.02%	0.003%
86	12.952	3688	3689	3690	rBV	290	101	0.01%	0.002%
87	13.032	3712	3714	3716	rBV2	349	142	0.02%	0.002%
88	13.501	3858	3860	3863	rVB2	811	321	0.04%	0.005%
89	14.498	4168	4170	4171	rVB2	431	89	0.01%	0.001%


Sum of corrected areas: 6057097

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014623.D
Acq On : 20 Feb 2020 15:03
Operator : SY/MD
Sample : L1584-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

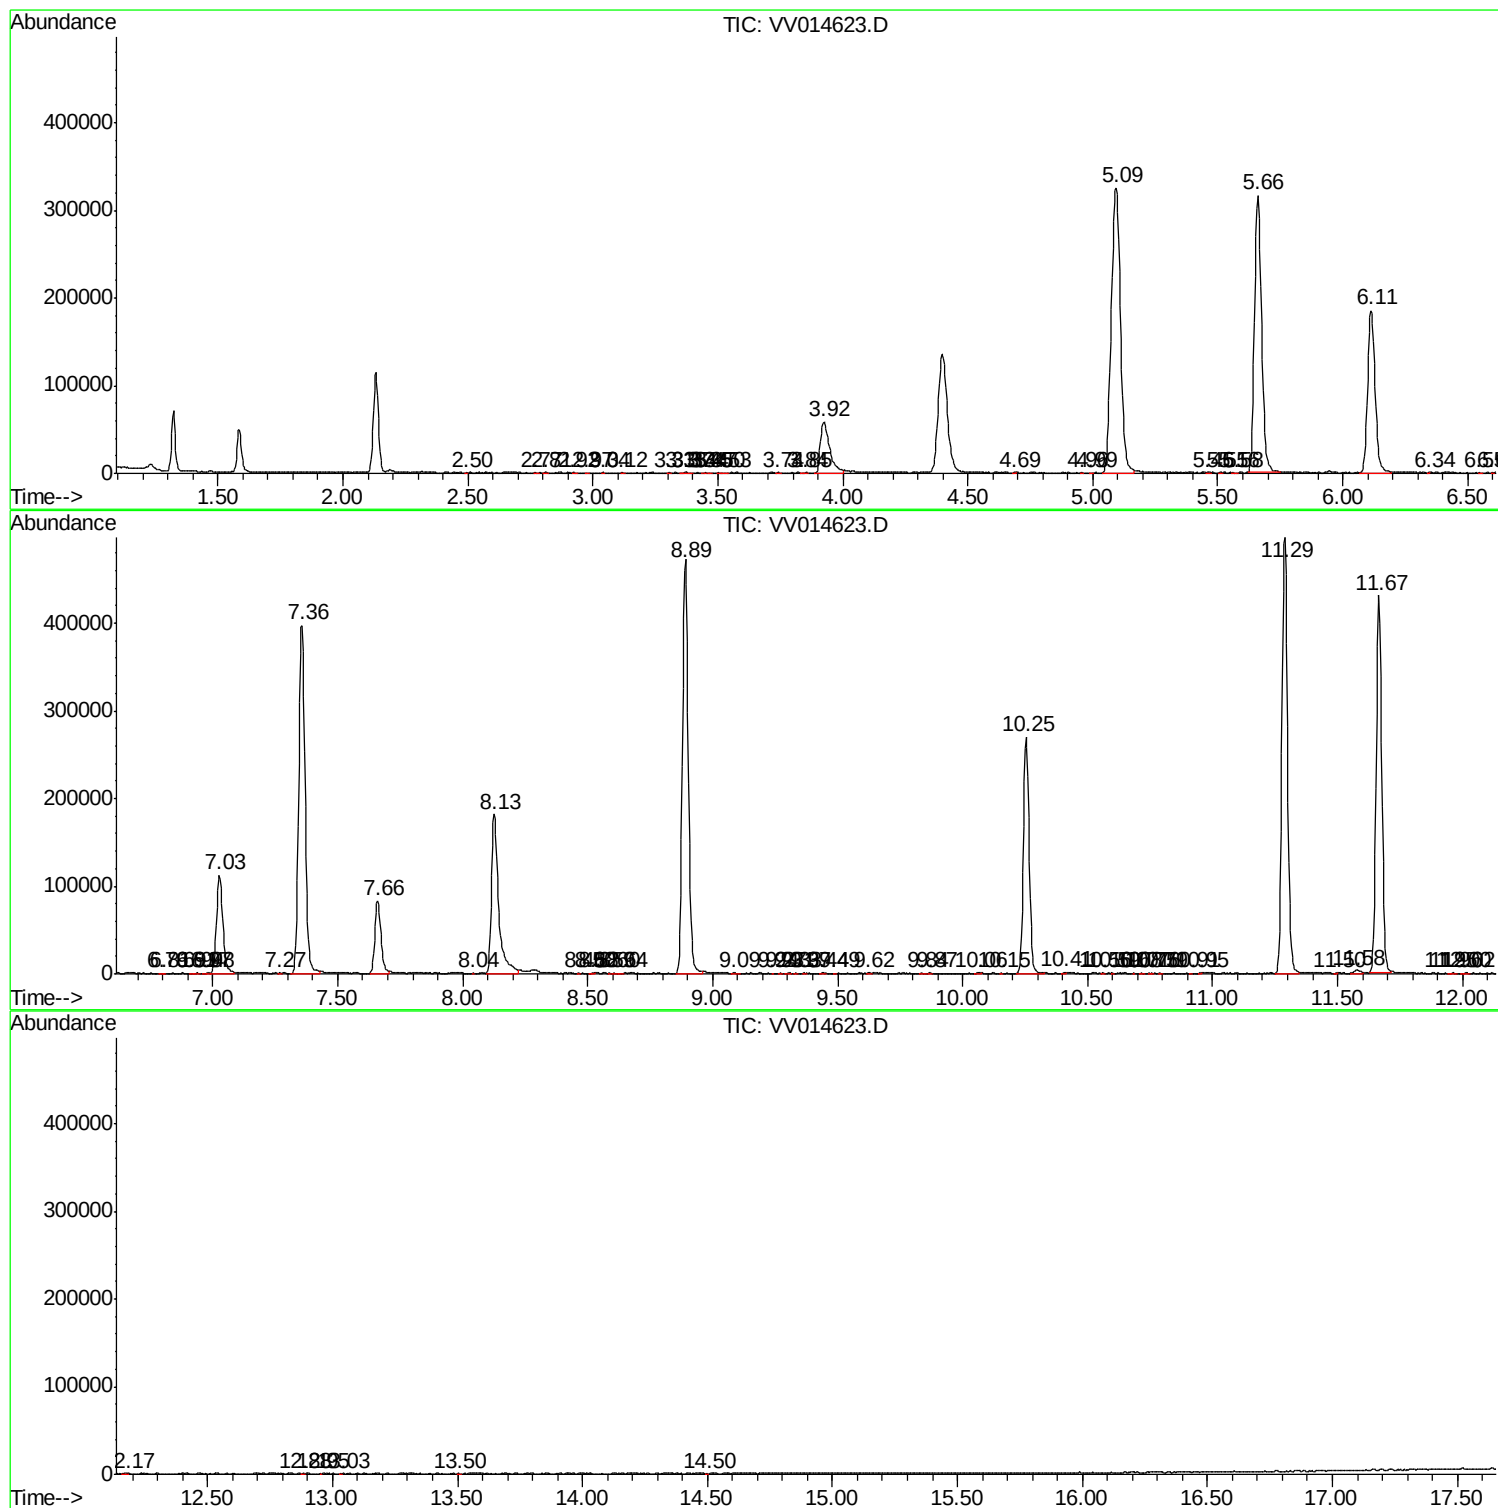

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV022020\
Data File : VV014623.D
Acq On : 20 Feb 2020 15:03
Operator : SY/MD
Sample : L1584-11
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AM7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014623.D
Acq On : 20 Feb 2020 15:03
Operator : SY/MD
Sample : L1584-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
