

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014624.D
 Acq On : 20 Feb 2020 15:27
 Operator : SY/MD
 Sample : L1607-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.476	430	431	436	rBV2	455	353	0.04%	0.006%
2	2.762	516	520	522	rVB2	562	375	0.05%	0.007%
3	2.884	554	558	562	rVB3	586	421	0.05%	0.007%
4	2.913	566	567	568	rBV3	212	50	0.01%	0.001%
5	2.994	589	592	594	rBV2	465	225	0.03%	0.004%
6	3.055	608	611	612	rBV2	299	141	0.02%	0.002%
7	3.081	616	619	622	rBV	459	334	0.04%	0.006%
8	3.174	645	648	651	rBV	312	199	0.03%	0.003%
9	3.203	655	657	658	rBV	269	107	0.01%	0.002%
10	3.235	665	667	668	rBV	184	88	0.01%	0.002%
11	3.383	708	713	717	rBV4	460	443	0.06%	0.008%
12	3.521	755	756	759	rBV	278	79	0.01%	0.001%
13	3.534	759	760	762	rBV	286	146	0.02%	0.003%
14	3.717	814	817	818	rBV2	344	172	0.02%	0.003%
15	3.769	830	833	834	rBV	274	125	0.02%	0.002%
16	3.775	834	835	836	rVV	322	74	0.01%	0.001%
17	3.827	849	851	852	rBV2	314	124	0.02%	0.002%
18	3.865	861	863	867	rVB2	427	235	0.03%	0.004%
19	3.881	867	868	869	rBV2	112	24	0.00%	0.000%
20	3.894	869	872	873	rBV	247	125	0.02%	0.002%
21	3.933	874	884	913	rBV	60010	169564	21.35%	2.940%
22	4.614	1094	1096	1100	rBV3	503	334	0.04%	0.006%
23	4.749	1134	1138	1143	rBV3	531	555	0.07%	0.010%
24	4.978	1206	1209	1211	rBV2	436	268	0.03%	0.005%
25	5.093	1228	1245	1265	rBV2	314064	794277	100.00%	13.769%
26	5.425	1344	1348	1351	rBV2	705	639	0.08%	0.011%
27	5.524	1375	1379	1381	rBV3	622	555	0.07%	0.010%
28	5.585	1396	1398	1402	rBV2	407	258	0.03%	0.004%
29	5.659	1409	1421	1450	rBV	292996	576811	72.62%	9.999%
30	6.013	1527	1531	1532	rBV	400	253	0.03%	0.004%
31	6.113	1550	1562	1584	rBV2	181686	363867	45.81%	6.308%
32	6.447	1662	1666	1672	rVB	457	462	0.06%	0.008%
33	6.476	1673	1675	1678	rVV	287	111	0.01%	0.002%
34	6.576	1703	1706	1709	rBV3	897	549	0.07%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014624.D
 Acq On : 20 Feb 2020 15:27
 Operator : SY/MD
 Sample : L1607-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

35	6.614	1715	1718	1721	rBV3	647	454	0.06%	0.008%
36	7.026	1836	1846	1866	rBV	111675	196404	24.73%	3.405%
37	7.309	1931	1934	1936	rBV2	371	224	0.03%	0.004%
38	7.357	1936	1949	1972	rBV	385504	677861	85.34%	11.751%
39	7.659	2033	2043	2070	rBV	78589	134557	16.94%	2.333%
40	7.871	2103	2109	2113	rBV5	826	945	0.12%	0.016%
41	8.129	2178	2189	2226	rBV	197516	365932	46.07%	6.344%
42	8.678	2357	2360	2363	rBV3	419	370	0.05%	0.006%
43	8.727	2373	2375	2378	rBV2	418	226	0.03%	0.004%
44	8.891	2414	2426	2452	rBV	430059	699096	88.02%	12.119%
45	9.103	2490	2492	2493	rBV	457	161	0.02%	0.003%
46	9.219	2525	2528	2532	rVB3	545	311	0.04%	0.005%
47	9.273	2542	2545	2546	rBV	345	183	0.02%	0.003%
48	9.360	2570	2572	2573	rBV	367	142	0.02%	0.002%
49	9.408	2586	2587	2591	rBV	251	189	0.02%	0.003%
50	9.556	2628	2633	2637	rBV2	550	491	0.06%	0.009%
51	9.794	2704	2707	2709	rBV2	230	120	0.02%	0.002%
52	9.833	2717	2719	2722	rBV2	448	242	0.03%	0.004%
53	9.955	2754	2757	2761	rBV4	432	365	0.05%	0.006%
54	10.000	2770	2771	2774	rBV	303	106	0.01%	0.002%
55	10.013	2774	2775	2778	rVB2	449	204	0.03%	0.004%
56	10.254	2839	2850	2870	rBV	254221	403185	50.76%	6.990%
57	10.466	2913	2916	2918	rBV3	394	241	0.03%	0.004%
58	10.778	3009	3013	3014	rBV2	383	272	0.03%	0.005%
59	10.813	3022	3024	3027	rBV2	343	107	0.01%	0.002%
60	10.829	3027	3029	3031	rBV	330	157	0.02%	0.003%
61	10.891	3045	3048	3049	rBV	343	179	0.02%	0.003%
62	10.916	3053	3056	3060	rBV2	439	378	0.05%	0.007%
63	11.074	3103	3105	3108	rBV2	384	230	0.03%	0.004%
64	11.289	3160	3172	3194	rBV	459705	716243	90.18%	12.417%
65	11.665	3278	3289	3307	rVB	411690	655845	82.57%	11.370%
66	11.839	3339	3343	3347	rBV4	458	457	0.06%	0.008%
67	12.325	3492	3494	3496	rBV	501	217	0.03%	0.004%


Sum of corrected areas: 5768437

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014624.D
Acq On : 20 Feb 2020 15:27
Operator : SY/MD
Sample : L1607-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

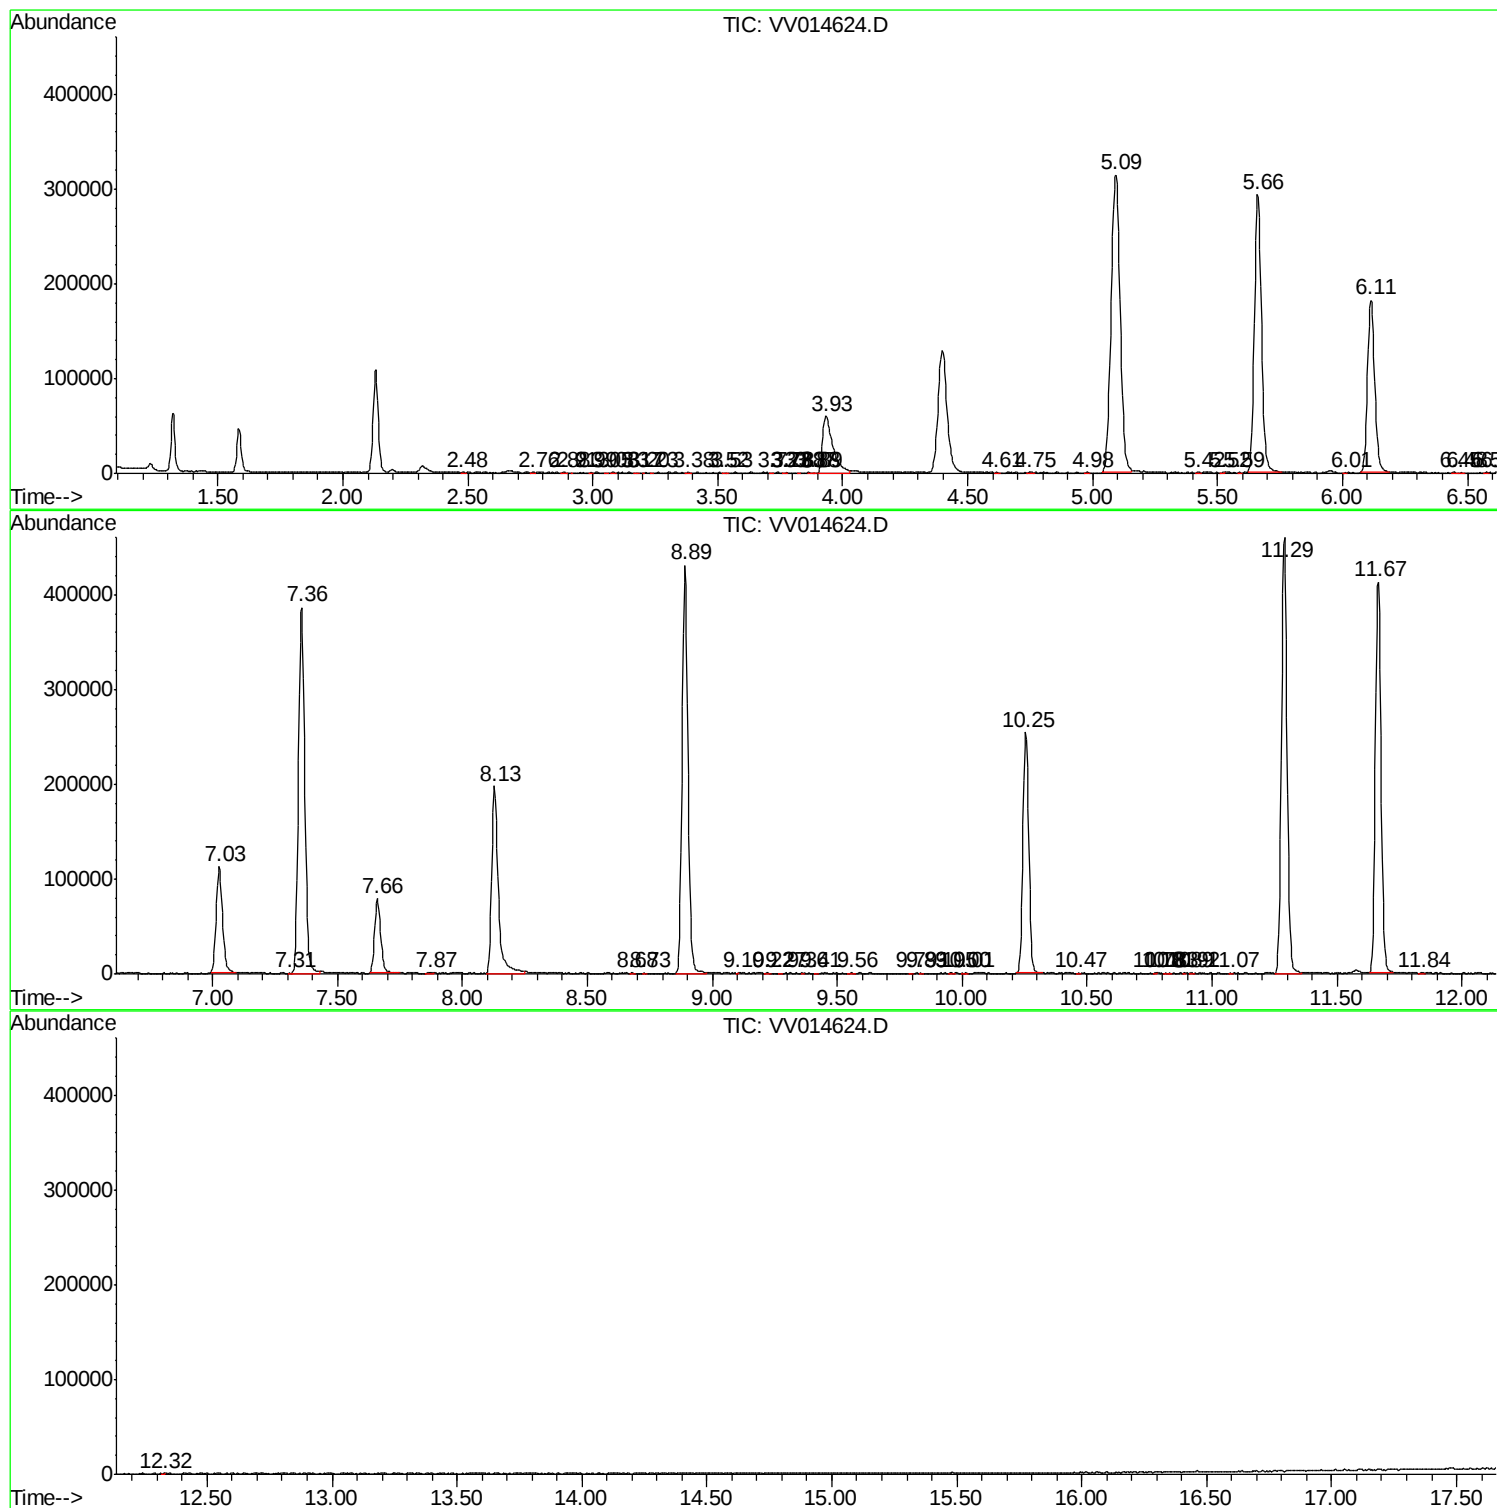

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014624.D
Acq On : 20 Feb 2020 15:27
Operator : SY/MD
Sample : L1607-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014624.D
Acq On : 20 Feb 2020 15:27
Operator : SY/MD
Sample : L1607-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc