

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014625.D
 Acq On : 20 Feb 2020 15:50
 Operator : SY/MD
 Sample : L1584-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.582	147	153	165	rVB	44438	52791	6.75%	0.860%
2	2.823	537	539	540	rBV	172	43	0.01%	0.001%
3	2.952	577	579	581	rBV2	432	111	0.01%	0.002%
4	3.421	724	725	730	rBV3	440	309	0.04%	0.005%
5	3.557	765	767	768	rBV	262	123	0.02%	0.002%
6	3.595	776	779	780	rBV	186	98	0.01%	0.002%
7	3.685	805	807	812	rBV	182	108	0.01%	0.002%
8	3.714	814	816	820	rBV2	468	337	0.04%	0.005%
9	3.778	832	836	837	rBV	233	174	0.02%	0.003%
10	3.823	846	850	851	rBV	386	196	0.03%	0.003%
11	3.929	873	883	909	rBV	54443	145229	18.57%	2.366%
12	4.396	1012	1028	1056	rBV	126565	324269	41.46%	5.282%
13	4.611	1094	1095	1099	rVB2	238	79	0.01%	0.001%
14	4.634	1100	1102	1104	rBV3	324	170	0.02%	0.003%
15	4.672	1112	1114	1115	rBV3	379	114	0.01%	0.002%
16	4.682	1115	1117	1119	rVB	248	86	0.01%	0.001%
17	4.785	1148	1149	1150	rVB	320	62	0.01%	0.001%
18	4.798	1150	1153	1154	rBV2	448	243	0.03%	0.004%
19	4.823	1160	1161	1162	rBV2	235	77	0.01%	0.001%
20	4.846	1166	1168	1169	rVB2	270	74	0.01%	0.001%
21	4.917	1185	1190	1191	rBV	219	206	0.03%	0.003%
22	4.981	1209	1210	1214	rBV	435	266	0.03%	0.004%
23	5.003	1214	1217	1219	rVB2	363	156	0.02%	0.003%
24	5.019	1221	1222	1224	rVB2	348	71	0.01%	0.001%
25	5.093	1225	1245	1279	rBV2	306347	782082	100.00%	12.739%
26	5.357	1325	1327	1335	rVB2	679	606	0.08%	0.010%
27	5.392	1335	1338	1342	rVB3	636	384	0.05%	0.006%
28	5.412	1342	1344	1346	rBV2	333	193	0.02%	0.003%
29	5.499	1369	1371	1372	rVB	313	115	0.01%	0.002%
30	5.524	1376	1379	1382	rBV3	646	521	0.07%	0.008%
31	5.566	1385	1392	1394	rBV3	609	458	0.06%	0.007%
32	5.659	1408	1421	1442	rBV	314212	618381	79.07%	10.072%
33	5.949	1503	1511	1514	rBV3	1947	2486	0.32%	0.040%
34	6.007	1526	1529	1531	rBV2	211	108	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014625.D
 Acq On : 20 Feb 2020 15:50
 Operator : SY/MD
 Sample : L1584-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

35	6.045	1536	1541	1542	rBV2	726	468	0.06%	0.008%
36	6.113	1546	1562	1591	rBV	175153	355490	45.45%	5.790%
37	6.402	1649	1652	1653	rBV	175	89	0.01%	0.001%
38	6.428	1658	1660	1662	rBV	419	235	0.03%	0.004%
39	6.502	1681	1683	1685	rVB2	502	210	0.03%	0.003%
40	6.553	1696	1699	1701	rBV2	449	289	0.04%	0.005%
41	6.611	1714	1717	1720	rBV2	448	226	0.03%	0.004%
42	6.643	1724	1727	1728	rBV2	515	238	0.03%	0.004%
43	6.714	1747	1749	1750	rBV	357	163	0.02%	0.003%
44	6.804	1775	1777	1779	rBV	318	111	0.01%	0.002%
45	6.868	1795	1797	1801	rBV	256	188	0.02%	0.003%
46	6.891	1801	1804	1805	rVB	358	134	0.02%	0.002%
47	6.965	1823	1827	1829	rBV3	522	403	0.05%	0.007%
48	7.026	1834	1846	1865	rBV2	109399	193228	24.71%	3.147%
49	7.273	1921	1923	1926	rBV2	381	231	0.03%	0.004%
50	7.357	1937	1949	1969	rBV	375625	651394	83.29%	10.610%
51	7.518	1996	1999	2002	rBV2	610	565	0.07%	0.009%
52	7.659	2033	2043	2069	rBV	78356	131782	16.85%	2.146%
53	7.820	2091	2093	2098	rBV3	588	409	0.05%	0.007%
54	7.900	2116	2118	2122	rVB3	823	484	0.06%	0.008%
55	8.035	2158	2160	2161	rBV2	379	205	0.03%	0.003%
56	8.061	2165	2168	2169	rBV2	453	197	0.03%	0.003%
57	8.129	2179	2189	2218	rBV	187195	341330	43.64%	5.560%
58	8.707	2366	2369	2372	rBV2	412	295	0.04%	0.005%
59	8.891	2415	2426	2443	rBV	454170	737595	94.31%	12.014%
60	9.232	2530	2532	2534	rBV2	235	119	0.02%	0.002%
61	9.379	2573	2578	2579	rBV2	232	164	0.02%	0.003%
62	9.460	2599	2603	2607	rVB2	430	317	0.04%	0.005%
63	9.569	2633	2637	2638	rBV	253	127	0.02%	0.002%
64	9.588	2638	2643	2644	rVV2	304	197	0.03%	0.003%
65	9.752	2690	2694	2695	rBV	381	217	0.03%	0.004%
66	9.823	2712	2716	2717	rBV	341	189	0.02%	0.003%
67	9.881	2732	2734	2737	rVB	390	179	0.02%	0.003%
68	9.897	2737	2739	2740	rBV2	387	177	0.02%	0.003%
69	9.955	2755	2757	2759	rBV	246	106	0.01%	0.002%
70	9.974	2759	2763	2764	rBV	421	276	0.04%	0.004%
71	10.026	2778	2779	2780	rBV	107	22	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014625.D
 Acq On : 20 Feb 2020 15:50
 Operator : SY/MD
 Sample : L1584-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

72	10.116	2805	2807	2809	rVB	594	190	0.02%	0.003%
73	10.177	2823	2826	2828	rBV	206	108	0.01%	0.002%
74	10.254	2838	2850	2866	rBV	251750	398436	50.95%	6.490%
75	10.537	2936	2938	2940	rBV	506	204	0.03%	0.003%
76	10.579	2949	2951	2958	rVB3	577	390	0.05%	0.006%
77	10.791	3015	3017	3020	rBV2	519	253	0.03%	0.004%
78	10.878	3042	3044	3045	rBV	242	86	0.01%	0.001%
79	10.965	3067	3071	3073	rBV	836	535	0.07%	0.009%
80	11.067	3099	3103	3104	rBV	322	181	0.02%	0.003%
81	11.289	3159	3172	3191	rBV	487410	763032	97.56%	12.428%
82	11.505	3238	3239	3241	rBV	275	150	0.02%	0.002%
83	11.534	3247	3248	3250	rBV	318	106	0.01%	0.002%
84	11.665	3278	3289	3303	rBV	397715	626463	80.10%	10.204%
85	12.627	3586	3588	3590	rBV	374	175	0.02%	0.003%
86	12.755	3626	3628	3629	rBV	233	69	0.01%	0.001%
87	13.981	4008	4009	4013	rBV	339	265	0.03%	0.004%


Sum of corrected areas: 6139418

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014625.D
Acq On : 20 Feb 2020 15:50
Operator : SY/MD
Sample : L1584-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0AM4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

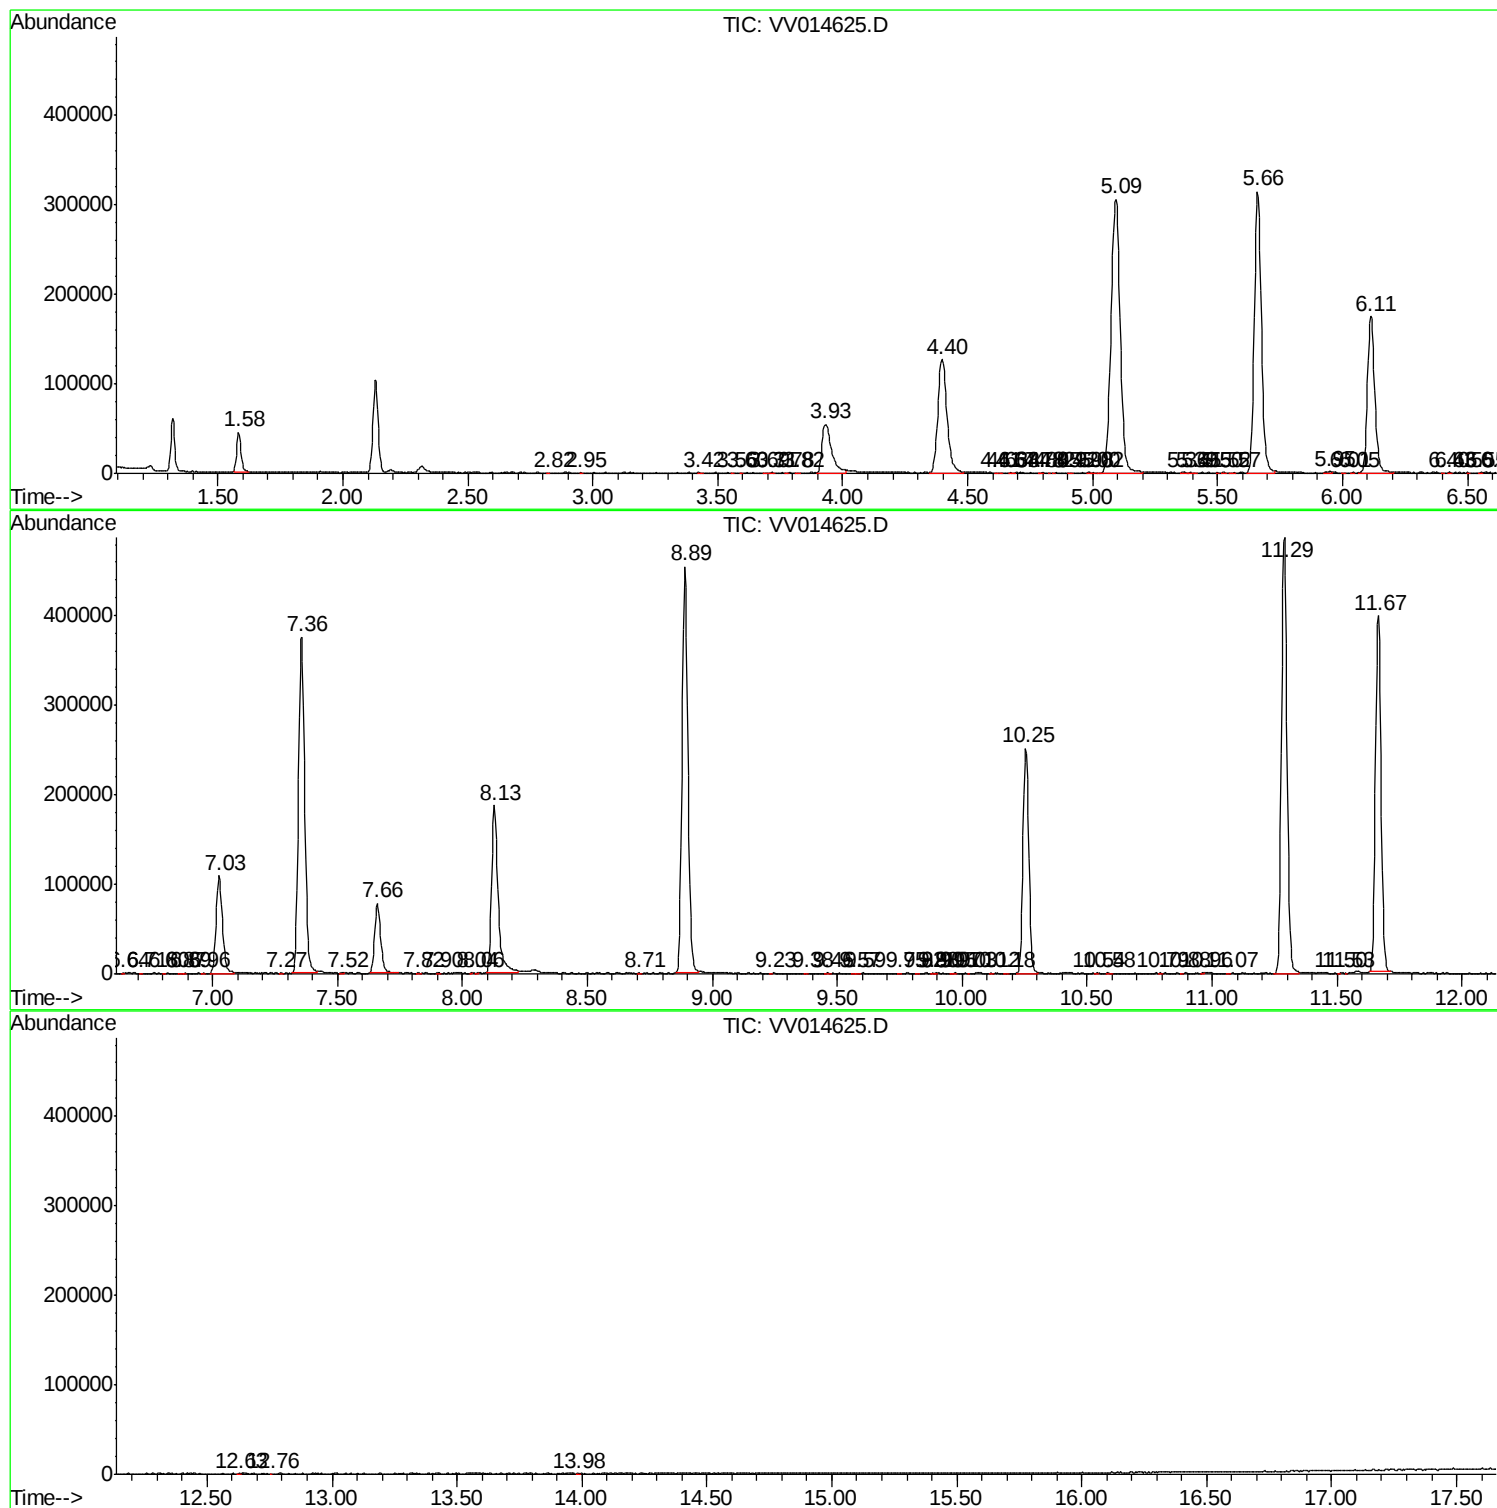

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014625.D
Acq On : 20 Feb 2020 15:50
Operator : SY/MD
Sample : L1584-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014625.D
Acq On : 20 Feb 2020 15:50
Operator : SY/MD
Sample : L1584-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc