

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014626.D
 Acq On : 20 Feb 2020 16:13
 Operator : SY/MD
 Sample : L1607-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	85	rVB	94965	95206	0.15%	0.140%
2	2.129	314	323	337	rBV2	172608	272658	0.44%	0.401%
3	2.884	553	558	562	rBV2	384	401	0.00%	0.001%
4	2.907	563	565	567	rBV2	512	244	0.00%	0.000%
5	2.984	587	589	592	rBV2	519	192	0.00%	0.000%
6	3.023	598	601	603	rBV3	506	276	0.00%	0.000%
7	3.126	631	633	634	rBV3	299	133	0.00%	0.000%
8	3.203	655	657	658	rBV	513	194	0.00%	0.000%
9	3.290	682	684	686	rBV2	429	183	0.00%	0.000%
10	3.370	707	709	711	rVB	272	90	0.00%	0.000%
11	3.399	717	718	719	rBV	293	60	0.00%	0.000%
12	3.434	725	729	731	rBV	374	303	0.00%	0.000%
13	3.508	750	752	754	rBV	299	105	0.00%	0.000%
14	3.537	759	761	763	rBV	200	63	0.00%	0.000%
15	3.691	807	809	811	rBV	257	90	0.00%	0.000%
16	3.759	829	830	832	rVB	392	142	0.00%	0.000%
17	3.785	836	838	839	rBV	399	128	0.00%	0.000%
18	3.814	846	847	852	rBV2	380	266	0.00%	0.000%
19	3.862	860	862	864	rVB	179	53	0.00%	0.000%
20	3.878	865	867	872	rVB	558	267	0.00%	0.000%
21	3.955	874	891	911	rBV2	93530	308065	0.50%	0.453%
22	4.791	1146	1151	1152	rBV	248	186	0.00%	0.000%
23	4.945	1195	1199	1201	rBV2	475	294	0.00%	0.000%
24	4.981	1209	1210	1213	rBV2	301	187	0.00%	0.000%
25	5.093	1228	1245	1281	rBV2	367618	937864	1.52%	1.379%
26	5.325	1314	1317	1320	rBV3	635	428	0.00%	0.001%
27	5.360	1325	1328	1331	rBV3	659	420	0.00%	0.001%
28	5.376	1331	1333	1335	rBV2	363	114	0.00%	0.000%
29	5.495	1368	1370	1373	rBV2	417	266	0.00%	0.000%
30	5.659	1408	1421	1448	rBV	299698	599012	0.97%	0.881%
31	5.884	1486	1491	1494	rBV3	556	407	0.00%	0.001%
32	5.974	1495	1519	1550	rBV	27830170	61639096	100.00%	90.610%
33	6.936	1816	1818	1820	rBV	455	138	0.00%	0.000%
34	7.026	1837	1846	1861	rVB2	129519	219682	0.36%	0.323%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014626.D
 Acq On : 20 Feb 2020 16:13
 Operator : SY/MD
 Sample : L1607-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

35	7.354	1936	1948	1965	rBV	454612	798012	1.29%	1.173%
36	7.617	2029	2030	2032	rBV2	388	120	0.00%	0.000%
37	7.659	2032	2043	2063	rBV	93536	157590	0.26%	0.232%
38	8.129	2179	2189	2218	rBV	206095	378988	0.61%	0.557%
39	8.453	2287	2290	2291	rBV3	577	288	0.00%	0.000%
40	8.521	2308	2311	2315	rBV2	414	283	0.00%	0.000%
41	8.566	2323	2325	2332	rVB3	416	453	0.00%	0.001%
42	8.592	2332	2333	2334	rBV	247	75	0.00%	0.000%
43	8.640	2346	2348	2350	rBV	301	141	0.00%	0.000%
44	8.733	2374	2377	2379	rBV2	391	249	0.00%	0.000%
45	8.891	2414	2426	2447	rBV	438672	707852	1.15%	1.041%
46	9.373	2574	2576	2578	rBV2	574	323	0.00%	0.000%
47	9.537	2624	2627	2629	rBV3	459	236	0.00%	0.000%
48	9.672	2666	2669	2672	rBV2	383	249	0.00%	0.000%
49	9.852	2723	2725	2727	rVB2	350	95	0.00%	0.000%
50	9.891	2735	2737	2740	rBV	455	195	0.00%	0.000%
51	9.971	2752	2762	2771	rBV	4863	8342	0.01%	0.012%
52	10.022	2775	2778	2779	rBV	354	153	0.00%	0.000%
53	10.048	2784	2786	2788	rBV	385	213	0.00%	0.000%
54	10.254	2839	2850	2868	rVB	274852	433669	0.70%	0.637%
55	10.546	2938	2941	2944	rVB3	601	344	0.00%	0.001%
56	10.640	2968	2970	2976	rVB4	512	481	0.00%	0.001%
57	10.665	2976	2978	2980	rBV	443	213	0.00%	0.000%
58	10.743	3000	3002	3008	rBV3	391	329	0.00%	0.000%
59	10.826	3026	3028	3030	rBV	469	177	0.00%	0.000%
60	11.093	3109	3111	3112	rBV	569	207	0.00%	0.000%
61	11.116	3117	3118	3121	rVB2	497	189	0.00%	0.000%
62	11.132	3121	3123	3126	rBV2	300	216	0.00%	0.000%
63	11.164	3131	3133	3136	rBV2	274	135	0.00%	0.000%
64	11.202	3143	3145	3146	rBV	430	158	0.00%	0.000%
65	11.289	3160	3172	3190	rBV	464004	725900	1.18%	1.067%
66	11.665	3277	3289	3304	rBV	468234	730625	1.19%	1.074%
67	11.913	3364	3366	3368	rBV	447	269	0.00%	0.000%
68	11.952	3375	3378	3379	rBV	378	136	0.00%	0.000%
69	11.971	3382	3384	3390	rBV2	536	342	0.00%	0.001%
70	12.411	3517	3521	3523	rBV	512	342	0.00%	0.001%
71	12.479	3539	3542	3543	rBV	409	214	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014626.D
Acq On : 20 Feb 2020 16:13
Operator : SY/MD
Sample : L1607-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN5

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Title : VOC Analysis

72	12.524	3554	3556	3560	rBV2	649	393	0.00%	0.001%
73	12.694	3605	3609	3612	rBV2	435	358	0.00%	0.001%
74	12.836	3649	3653	3657	rBV2	399	431	0.00%	0.001%
75	13.463	3847	3848	3852	rBV2	348	203	0.00%	0.000%
76	13.511	3862	3863	3864	rBV	435	118	0.00%	0.000%
77	13.537	3869	3871	3872	rBV2	410	174	0.00%	0.000%


Sum of corrected areas: 68026693

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014626.D
Acq On : 20 Feb 2020 16:13
Operator : SY/MD
Sample : L1607-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

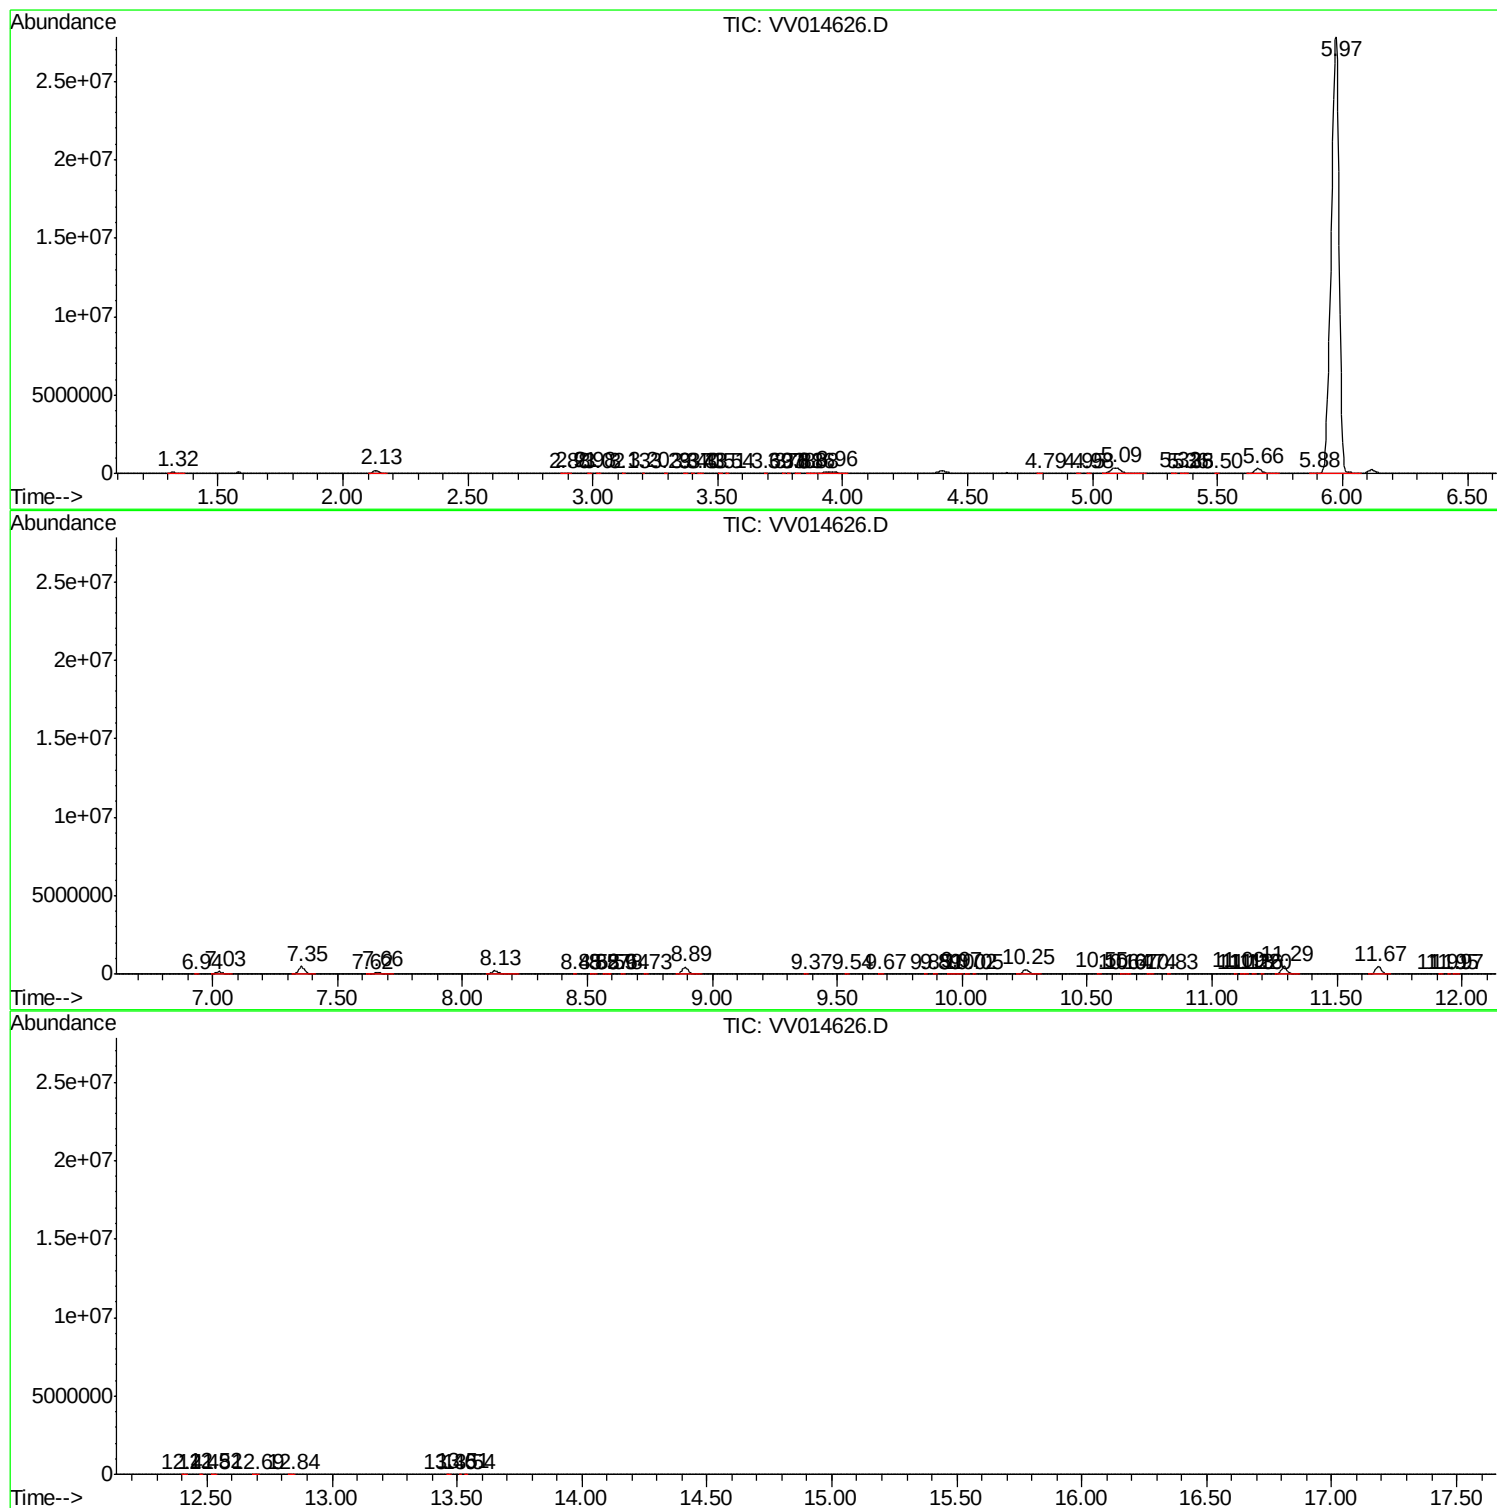

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014626.D
Acq On : 20 Feb 2020 16:13
Operator : SY/MD
Sample : L1607-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014626.D
Acq On : 20 Feb 2020 16:13
Operator : SY/MD
Sample : L1607-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc