

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014627.D
 Acq On : 20 Feb 2020 16:36
 Operator : SY/MD
 Sample : L1607-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.585	147	154	167	rVB	47385	56414	7.13%	0.895%
2	2.000	281	283	287	rVB3	785	481	0.06%	0.008%
3	2.132	314	324	339	rBV	107414	154460	19.53%	2.451%
4	2.756	514	518	523	rVB3	349	297	0.04%	0.005%
5	2.798	529	531	532	rBV	234	124	0.02%	0.002%
6	2.904	563	564	567	rBV	442	144	0.02%	0.002%
7	3.019	599	600	603	rBV	707	305	0.04%	0.005%
8	3.119	629	631	634	rBV	488	212	0.03%	0.003%
9	3.241	668	669	673	rBV2	350	191	0.02%	0.003%
10	3.418	722	724	727	rBV2	464	334	0.04%	0.005%
11	3.672	802	803	805	rBV	338	113	0.01%	0.002%
12	3.698	809	811	814	rVB3	399	251	0.03%	0.004%
13	3.939	875	886	922	rBV	53242	150472	19.02%	2.387%
14	4.608	1092	1094	1099	rBV4	470	343	0.04%	0.005%
15	4.788	1147	1150	1152	rBV	273	245	0.03%	0.004%
16	5.093	1222	1245	1269	rBV2	312907	791043	100.00%	12.550%
17	5.450	1353	1356	1357	rBV	644	395	0.05%	0.006%
18	5.556	1387	1389	1391	rBV	407	199	0.03%	0.003%
19	5.659	1408	1421	1444	rBV	313117	625319	79.05%	9.921%
20	5.958	1501	1514	1536	rBV	129541	253809	32.09%	4.027%
21	6.113	1547	1562	1583	rBV	178992	362719	45.85%	5.755%
22	6.350	1634	1636	1639	rBV2	427	199	0.03%	0.003%
23	6.444	1663	1665	1669	rVB2	231	142	0.02%	0.002%
24	6.466	1669	1672	1677	rBV3	493	379	0.05%	0.006%
25	6.598	1711	1713	1715	rBV	315	151	0.02%	0.002%
26	6.617	1717	1719	1721	rVB2	175	54	0.01%	0.001%
27	6.711	1746	1748	1751	rVB2	692	348	0.04%	0.006%
28	6.733	1752	1755	1758	rVV2	399	281	0.04%	0.004%
29	6.762	1760	1764	1766	rBV2	397	297	0.04%	0.005%
30	6.791	1770	1773	1774	rBV2	486	199	0.03%	0.003%
31	6.920	1810	1813	1815	rBV	482	246	0.03%	0.004%
32	7.026	1833	1846	1867	rBV	109309	196621	24.86%	3.119%
33	7.357	1935	1949	1974	rBV	382097	668751	84.54%	10.610%
34	7.659	2033	2043	2066	rBV	76994	135325	17.11%	2.147%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014627.D
 Acq On : 20 Feb 2020 16:36
 Operator : SY/MD
 Sample : L1607-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

35	7.865	2104	2107	2108	rBV	337	196	0.02%	0.003%
36	8.055	2165	2166	2168	rVB	501	185	0.02%	0.003%
37	8.129	2178	2189	2210	rBV	193059	350178	44.27%	5.556%
38	8.553	2319	2321	2324	rBV2	620	318	0.04%	0.005%
39	8.801	2396	2398	2401	rBV	299	140	0.02%	0.002%
40	8.839	2407	2410	2414	rVB2	328	244	0.03%	0.004%
41	8.891	2414	2426	2446	rBV	457692	747580	94.51%	11.861%
42	9.170	2512	2513	2515	rBV	496	199	0.03%	0.003%
43	9.347	2567	2568	2571	rBV	218	86	0.01%	0.001%
44	9.373	2573	2576	2577	rBV	395	170	0.02%	0.003%
45	9.408	2584	2587	2588	rBV	202	109	0.01%	0.002%
46	9.456	2601	2602	2604	rBV2	369	151	0.02%	0.002%
47	9.563	2633	2635	2639	rVB2	707	384	0.05%	0.006%
48	9.704	2676	2679	2682	rBV2	569	367	0.05%	0.006%
49	9.797	2704	2708	2711	rBV2	371	219	0.03%	0.003%
50	9.916	2740	2745	2748	rBV2	538	386	0.05%	0.006%
51	10.116	2805	2807	2812	rBV3	260	198	0.03%	0.003%
52	10.135	2812	2813	2816	rBV2	242	118	0.01%	0.002%
53	10.254	2839	2850	2870	rBV	259799	400482	50.63%	6.354%
54	10.563	2944	2946	2948	rBV	313	122	0.02%	0.002%
55	10.572	2948	2949	2951	rBV	233	109	0.01%	0.002%
56	10.794	3014	3018	3021	rBV2	373	326	0.04%	0.005%
57	11.099	3111	3113	3116	rBV	379	210	0.03%	0.003%
58	11.135	3123	3124	3127	rBV	242	134	0.02%	0.002%
59	11.289	3160	3172	3191	rBV	487099	758050	95.83%	12.027%
60	11.665	3278	3289	3311	rVB	405573	640943	81.03%	10.169%
61	11.907	3361	3364	3365	rBV	316	169	0.02%	0.003%
62	12.173	3445	3447	3448	rBV	291	80	0.01%	0.001%
63	13.408	3828	3831	3832	rBV	502	273	0.03%	0.004%


Sum of corrected areas: 6302989

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014627.D
Acq On : 20 Feb 2020 16:36
Operator : SY/MD
Sample : L1607-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

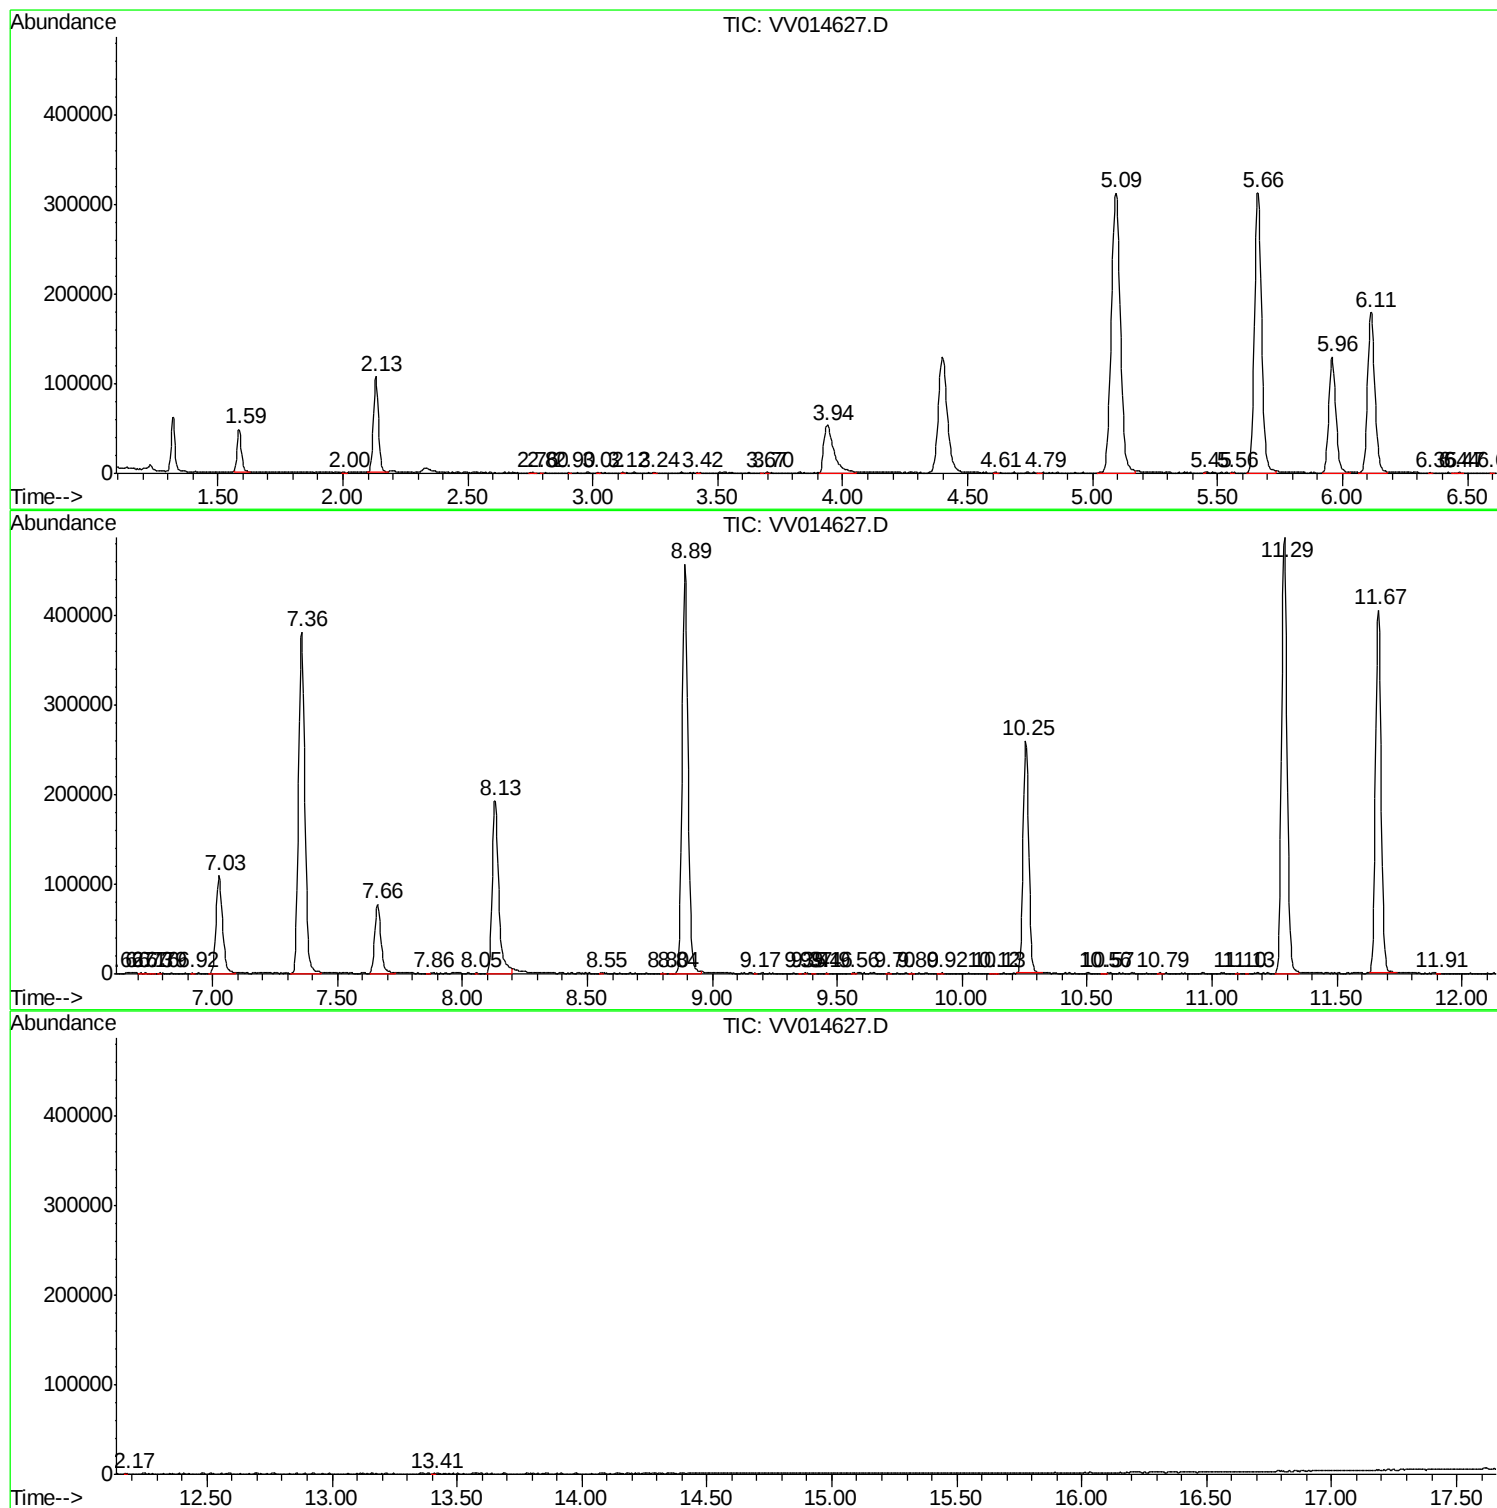

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014627.D
Acq On : 20 Feb 2020 16:36
Operator : SY/MD
Sample : L1607-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014627.D
Acq On : 20 Feb 2020 16:36
Operator : SY/MD
Sample : L1607-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc