

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014628.D
 Acq On : 20 Feb 2020 16:59
 Operator : SY/MD
 Sample : L1607-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.582	147	153	166	rBV	44383	53538	2.62%	0.713%
2	2.608	470	472	474	rBV	430	151	0.01%	0.002%
3	2.749	514	516	520	rBV2	520	353	0.02%	0.005%
4	2.936	572	574	576	rBV	341	190	0.01%	0.003%
5	2.961	580	582	586	rBV3	478	244	0.01%	0.003%
6	3.090	621	622	625	rVB	332	150	0.01%	0.002%
7	3.148	638	640	643	rBV	360	191	0.01%	0.003%
8	3.164	643	645	646	rBV	307	102	0.01%	0.001%
9	3.318	689	693	694	rBV2	448	244	0.01%	0.003%
10	3.453	732	735	738	rBV2	529	276	0.01%	0.004%
11	3.479	742	743	746	rVB	214	69	0.00%	0.001%
12	3.508	749	752	756	rBV2	388	283	0.01%	0.004%
13	3.531	757	759	761	rVB	293	117	0.01%	0.002%
14	3.637	790	792	794	rVB2	439	178	0.01%	0.002%
15	3.653	794	797	800	rBV3	500	418	0.02%	0.006%
16	3.746	824	826	828	rVB2	499	191	0.01%	0.003%
17	3.762	828	831	835	rBV3	631	404	0.02%	0.005%
18	3.836	852	854	856	rVB	152	39	0.00%	0.001%
19	3.852	857	859	862	rBV2	321	206	0.01%	0.003%
20	3.894	870	872	873	rBV	224	66	0.00%	0.001%
21	3.936	874	885	907	rBV	55159	143999	7.06%	1.918%
22	4.723	1128	1130	1136	rVB3	634	421	0.02%	0.006%
23	4.772	1144	1145	1146	rVB3	189	36	0.00%	0.000%
24	4.826	1160	1162	1166	rVB2	438	243	0.01%	0.003%
25	4.846	1166	1168	1170	rBV2	408	202	0.01%	0.003%
26	4.904	1184	1186	1187	rBV	286	141	0.01%	0.002%
27	4.945	1197	1199	1202	rBV2	334	171	0.01%	0.002%
28	4.984	1207	1211	1214	rBV2	409	318	0.02%	0.004%
29	5.029	1223	1225	1226	rBV	563	192	0.01%	0.003%
30	5.093	1227	1245	1273	rBV2	312120	787777	38.62%	10.493%
31	5.402	1337	1341	1342	rBV2	559	389	0.02%	0.005%
32	5.495	1366	1370	1373	rBV3	335	268	0.01%	0.004%
33	5.511	1373	1375	1377	rBV	442	216	0.01%	0.003%
34	5.556	1386	1389	1391	rVB2	355	195	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014628.D
 Acq On : 20 Feb 2020 16:59
 Operator : SY/MD
 Sample : L1607-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

35	5.572	1391	1394	1395	rBV2	398	146	0.01%	0.002%
36	5.659	1408	1421	1447	rBV	308324	612647	30.04%	8.160%
37	5.855	1480	1482	1484	rBV	247	143	0.01%	0.002%
38	5.958	1499	1514	1541	rBV	1049453	2039755	100.00%	27.169%
39	6.293	1616	1618	1619	rBV2	742	271	0.01%	0.004%
40	6.386	1643	1647	1649	rBB2	331	236	0.01%	0.003%
41	6.473	1673	1674	1676	rVB	309	63	0.00%	0.001%
42	6.492	1676	1680	1683	rVB2	571	321	0.02%	0.004%
43	6.505	1683	1684	1685	rBV2	96	25	0.00%	0.000%
44	6.514	1685	1687	1690	rBV4	519	257	0.01%	0.003%
45	6.543	1694	1696	1700	rVB2	278	178	0.01%	0.002%
46	6.569	1700	1704	1706	rBV2	392	225	0.01%	0.003%
47	6.608	1714	1716	1718	rBV2	289	162	0.01%	0.002%
48	6.701	1743	1745	1747	rBV	213	134	0.01%	0.002%
49	6.714	1747	1749	1750	rBV	369	182	0.01%	0.002%
50	6.836	1784	1787	1789	rBV2	497	337	0.02%	0.004%
51	7.026	1834	1846	1863	rBV	109348	194795	9.55%	2.595%
52	7.280	1921	1925	1929	rBV4	537	601	0.03%	0.008%
53	7.357	1936	1949	1967	rBV	379669	662556	32.48%	8.825%
54	7.659	2034	2043	2065	rBV	78028	129036	6.33%	1.719%
55	7.981	2135	2143	2149	rBV4	763	1318	0.06%	0.018%
56	8.061	2165	2168	2171	rBV2	203	139	0.01%	0.002%
57	8.080	2171	2174	2176	rBV3	346	182	0.01%	0.002%
58	8.128	2179	2189	2221	rVV	189827	348780	17.10%	4.646%
59	8.508	2303	2307	2308	rBV2	668	338	0.02%	0.005%
60	8.646	2348	2350	2352	rBV2	557	253	0.01%	0.003%
61	8.675	2357	2359	2363	rVB2	307	97	0.00%	0.001%
62	8.694	2363	2365	2367	rBV2	471	196	0.01%	0.003%
63	8.833	2406	2408	2411	rBV	386	255	0.01%	0.003%
64	8.890	2415	2426	2444	rVV	457108	734757	36.02%	9.787%
65	9.093	2487	2489	2490	rBV	371	124	0.01%	0.002%
66	9.235	2532	2533	2536	rBV2	399	253	0.01%	0.003%
67	9.318	2558	2559	2562	rVB2	346	136	0.01%	0.002%
68	9.585	2639	2642	2646	rBV2	502	331	0.02%	0.004%
69	9.662	2662	2666	2668	rBV2	411	272	0.01%	0.004%
70	9.688	2673	2674	2678	rBV2	202	83	0.00%	0.001%
71	9.752	2692	2694	2696	rBV2	389	168	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014628.D
 Acq On : 20 Feb 2020 16:59
 Operator : SY/MD
 Sample : L1607-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

72	9.804	2708	2710	2711	rBV	267	93	0.00%	0.001%
73	9.858	2725	2727	2732	rVB	363	182	0.01%	0.002%
74	9.968	2759	2761	2764	rBV	154	72	0.00%	0.001%
75	10.042	2781	2784	2785	rBV	403	239	0.01%	0.003%
76	10.254	2838	2850	2866	rBV	251547	397215	19.47%	5.291%
77	10.350	2879	2880	2883	rBV	274	176	0.01%	0.002%
78	10.479	2916	2920	2922	rBV2	632	376	0.02%	0.005%
79	10.582	2947	2952	2954	rBV	380	262	0.01%	0.003%
80	10.710	2991	2992	2996	rBV	243	163	0.01%	0.002%
81	10.816	3022	3025	3027	rBV2	289	125	0.01%	0.002%
82	10.929	3057	3060	3062	rBV2	460	248	0.01%	0.003%
83	11.093	3110	3111	3116	rBV2	508	388	0.02%	0.005%
84	11.289	3160	3172	3188	rBV	477055	748775	36.71%	9.973%
85	11.665	3278	3289	3310	rVB	397505	636777	31.22%	8.482%
86	11.868	3348	3352	3354	rBV2	417	286	0.01%	0.004%
87	12.251	3469	3471	3473	rBV	367	175	0.01%	0.002%
88	13.009	3704	3707	3709	rBV	433	283	0.01%	0.004%
89	13.151	3749	3751	3752	rBV	342	133	0.01%	0.002%
90	13.263	3785	3786	3787	rBV	237	83	0.00%	0.001%


Sum of corrected areas: 7507781

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014628.D
Acq On : 20 Feb 2020 16:59
Operator : SY/MD
Sample : L1607-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

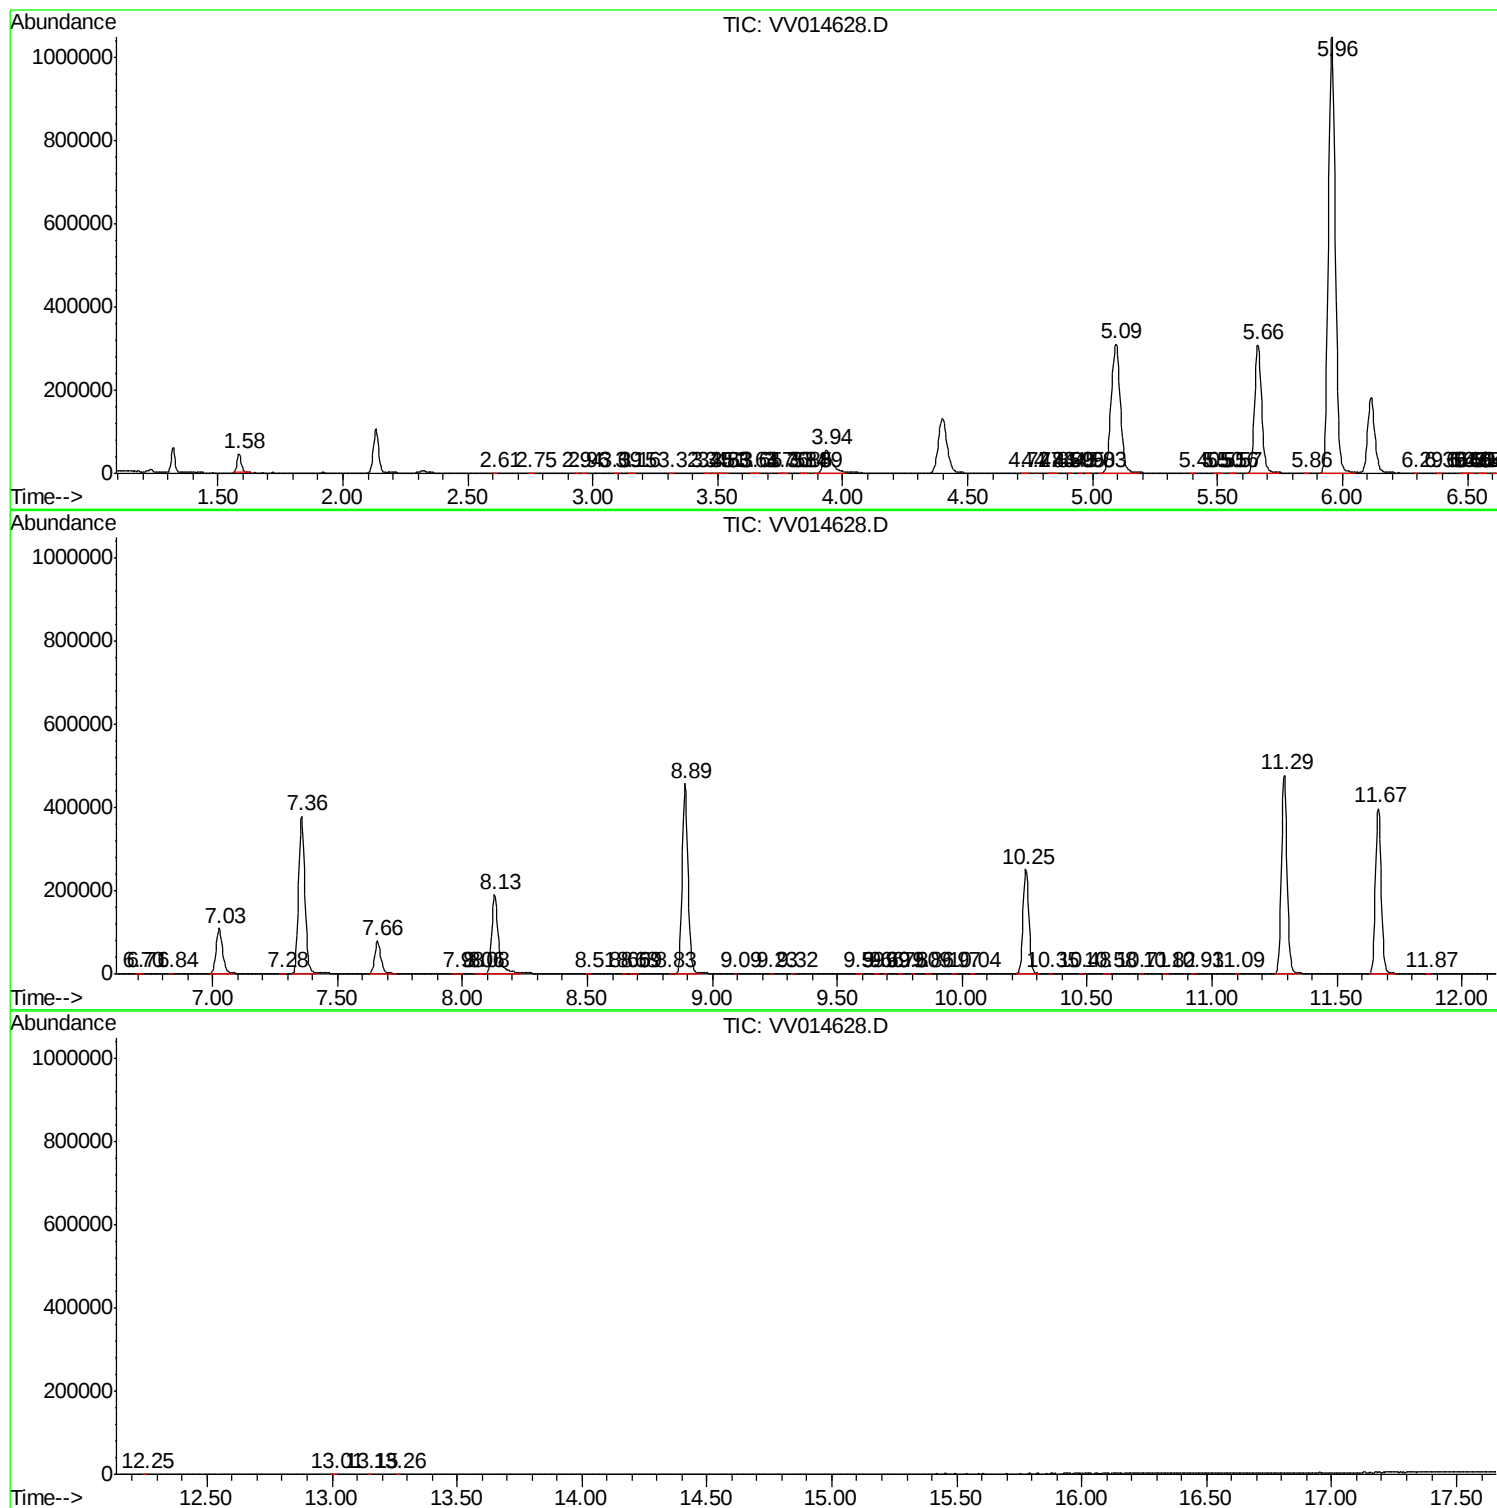

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014628.D
Acq On : 20 Feb 2020 16:59
Operator : SY/MD
Sample : L1607-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014628.D
Acq On : 20 Feb 2020 16:59
Operator : SY/MD
Sample : L1607-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc