

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014630.D
 Acq On : 20 Feb 2020 17:46
 Operator : SY/MD
 Sample : L1607-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	66	71	83	rVB	86894	89961	9.82%	1.485%
2	1.586	147	154	175	rVB	59535	76338	8.33%	1.260%
3	2.794	529	530	532	rBV	342	133	0.01%	0.002%
4	2.962	580	582	583	rBV	332	103	0.01%	0.002%
5	3.045	605	608	614	rBV3	560	584	0.06%	0.010%
6	3.409	720	721	723	rBV	394	175	0.02%	0.003%
7	3.466	738	739	742	rVB2	275	96	0.01%	0.002%
8	3.486	742	745	746	rBV	155	56	0.01%	0.001%
9	3.499	746	749	753	rBV2	526	322	0.04%	0.005%
10	3.547	762	764	765	rBV2	229	75	0.01%	0.001%
11	3.566	767	770	773	rVV2	288	177	0.02%	0.003%
12	3.685	806	807	810	rVB	252	119	0.01%	0.002%
13	3.737	822	823	827	rVB3	514	173	0.02%	0.003%
14	3.765	827	832	835	rBV2	374	283	0.03%	0.005%
15	3.859	859	861	862	rBV	179	75	0.01%	0.001%
16	3.888	868	870	874	rBV2	185	121	0.01%	0.002%
17	3.939	874	886	914	rBV	56584	161349	17.61%	2.663%
18	4.769	1142	1144	1146	rBV	451	181	0.02%	0.003%
19	4.782	1146	1148	1150	rBV	321	143	0.02%	0.002%
20	4.839	1162	1166	1168	rBV	515	376	0.04%	0.006%
21	4.868	1173	1175	1177	rBV	276	139	0.02%	0.002%
22	4.913	1187	1189	1193	rVB3	674	374	0.04%	0.006%
23	5.007	1216	1218	1221	rBV	350	171	0.02%	0.003%
24	5.093	1225	1245	1267	rBV2	365792	916318	100.00%	15.126%
25	5.312	1311	1313	1316	rBV2	475	223	0.02%	0.004%
26	5.360	1325	1328	1330	rBV3	515	349	0.04%	0.006%
27	5.482	1364	1366	1368	rBV	242	103	0.01%	0.002%
28	5.502	1370	1372	1374	rBV2	298	140	0.02%	0.002%
29	5.659	1407	1421	1440	rBV	306744	606021	66.14%	10.004%
30	5.849	1478	1480	1486	rVB4	613	400	0.04%	0.007%
31	5.872	1486	1487	1488	rBV	502	111	0.01%	0.002%
32	5.958	1502	1514	1530	rBV6	18764	40289	4.40%	0.665%
33	6.052	1540	1543	1547	rBV3	502	408	0.04%	0.007%
34	6.322	1624	1627	1630	rBV	358	208	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014630.D
 Acq On : 20 Feb 2020 17:46
 Operator : SY/MD
 Sample : L1607-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

35	6.396	1649	1650	1651	rBV	285	77	0.01%	0.001%
36	6.405	1651	1653	1654	rVB2	263	71	0.01%	0.001%
37	6.473	1669	1674	1676	rVB	407	300	0.03%	0.005%
38	6.556	1698	1700	1702	rBV	580	205	0.02%	0.003%
39	6.582	1707	1708	1711	rVB2	415	124	0.01%	0.002%
40	6.627	1717	1722	1725	rBV2	335	253	0.03%	0.004%
41	6.762	1762	1764	1765	rBV	317	112	0.01%	0.002%
42	6.855	1791	1793	1801	rVB2	496	399	0.04%	0.007%
43	6.888	1801	1803	1806	rVB3	221	113	0.01%	0.002%
44	6.907	1806	1809	1810	rBV3	264	117	0.01%	0.002%
45	6.926	1814	1815	1817	rBV2	322	123	0.01%	0.002%
46	6.955	1819	1824	1825	rBV2	506	300	0.03%	0.005%
47	7.026	1834	1846	1866	rBV	125102	222217	24.25%	3.668%
48	7.283	1924	1926	1929	rVB	227	106	0.01%	0.002%
49	7.296	1929	1930	1933	rBV	221	120	0.01%	0.002%
50	7.357	1936	1949	1970	rBV	445492	779500	85.07%	12.868%
51	7.614	2025	2029	2030	rBV2	269	123	0.01%	0.002%
52	7.659	2032	2043	2062	rBV	90822	152075	16.60%	2.510%
53	8.084	2171	2175	2176	rBV2	198	108	0.01%	0.002%
54	8.132	2180	2190	2217	rVV	206043	376981	41.14%	6.223%
55	8.441	2285	2286	2287	rBV	180	56	0.01%	0.001%
56	8.524	2310	2312	2313	rBV	279	100	0.01%	0.002%
57	8.582	2326	2330	2332	rBV3	446	375	0.04%	0.006%
58	8.691	2359	2364	2366	rVB	374	326	0.04%	0.005%
59	8.704	2366	2368	2369	rBV	192	67	0.01%	0.001%
60	8.765	2385	2387	2389	rBV	259	136	0.01%	0.002%
61	8.891	2413	2426	2444	rBV	454013	733796	80.08%	12.113%
62	9.248	2535	2537	2538	rBV	203	93	0.01%	0.002%
63	9.360	2571	2572	2574	rVB2	318	103	0.01%	0.002%
64	9.396	2580	2583	2584	rBV2	213	102	0.01%	0.002%
65	9.559	2630	2634	2635	rBV3	440	270	0.03%	0.004%
66	9.913	2741	2744	2745	rBV	301	141	0.02%	0.002%
67	10.254	2838	2850	2867	rBV	273121	432676	47.22%	7.142%
68	10.476	2917	2919	2920	rBV2	344	105	0.01%	0.002%
69	10.649	2970	2973	2975	rBV	314	194	0.02%	0.003%
70	10.772	3008	3011	3015	rBV	492	274	0.03%	0.005%
71	10.846	3031	3034	3037	rBV2	347	301	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014630.D
Acq On : 20 Feb 2020 17:46
Operator : SY/MD
Sample : L1607-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Title : VOC Analysis

72	11.238	3152	3156	3160	rBV3	525	441	0.05%	0.007%
73	11.289	3160	3172	3191	rBV	474561	738176	80.56%	12.185%
74	11.569	3258	3259	3263	rBV2	441	301	0.03%	0.005%
75	11.666	3277	3289	3311	rBV	453402	718878	78.45%	11.867%
76	11.871	3349	3353	3356	rBV2	655	467	0.05%	0.008%
77	12.476	3539	3541	3543	rBV	337	143	0.02%	0.002%
78	12.537	3557	3560	3563	rBV3	444	302	0.03%	0.005%
79	12.846	3653	3656	3659	rBV2	754	515	0.06%	0.009%


Sum of corrected areas: 6057856

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014630.D
Acq On : 20 Feb 2020 17:46
Operator : SY/MD
Sample : L1607-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

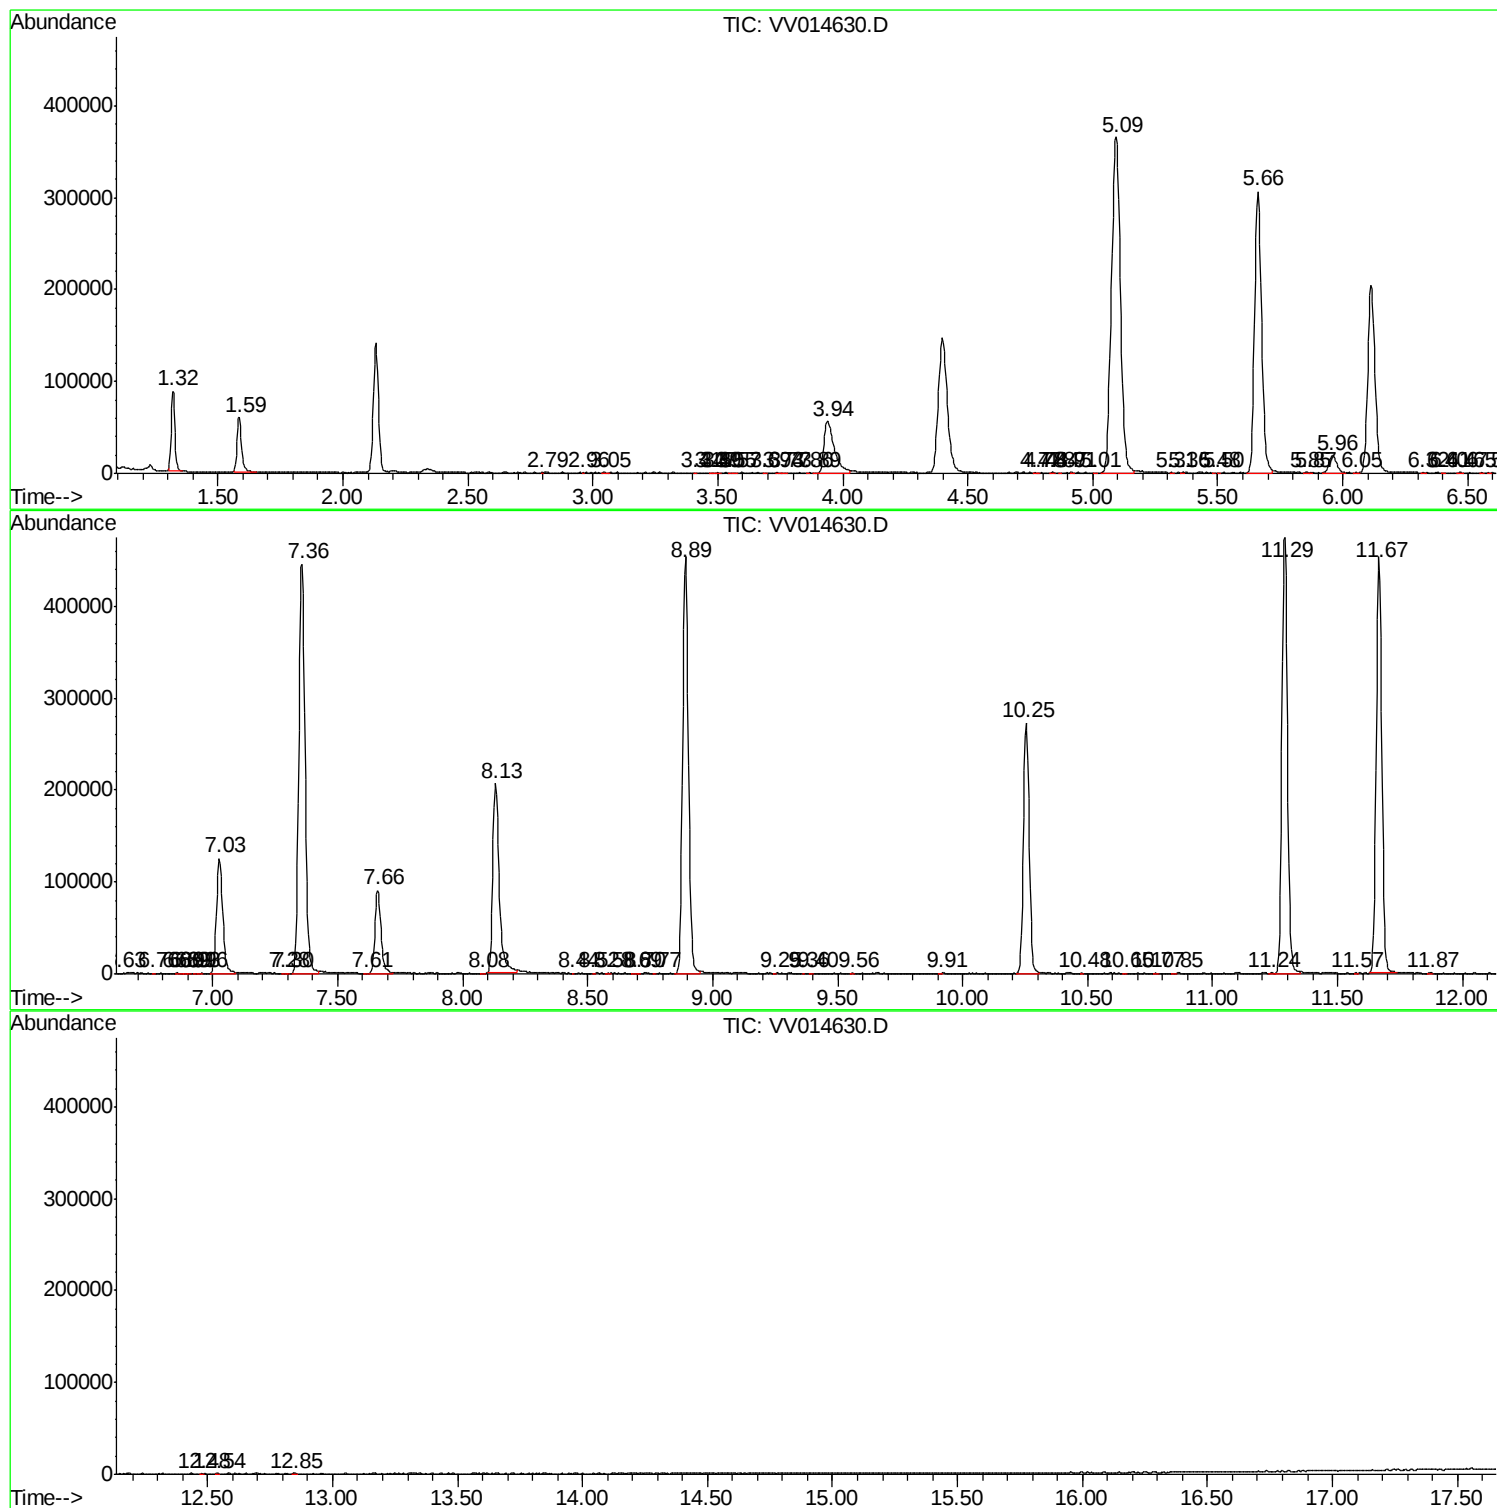

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014630.D
Acq On : 20 Feb 2020 17:46
Operator : SY/MD
Sample : L1607-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014630.D
Acq On : 20 Feb 2020 17:46
Operator : SY/MD
Sample : L1607-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc