

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014636.D
 Acq On : 20 Feb 2020 20:07
 Operator : SY/MD
 Sample : L1607-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	82	rVB	83864	86351	9.66%	1.257%
2	1.582	147	153	170	rVB	56338	69406	7.77%	1.011%
3	1.756	201	207	211	rBV5	966	1144	0.13%	0.017%
4	1.981	276	277	280	rBV2	647	379	0.04%	0.006%
5	2.132	313	324	336	rBV	140608	203826	22.81%	2.968%
6	3.213	659	660	662	rBV2	279	102	0.01%	0.001%
7	3.344	698	701	703	rBV2	404	173	0.02%	0.003%
8	3.444	730	732	735	rBV2	327	143	0.02%	0.002%
9	3.467	735	739	742	rVV2	466	372	0.04%	0.005%
10	3.537	757	761	764	rBV	303	266	0.03%	0.004%
11	3.598	775	780	783	rBV3	490	390	0.04%	0.006%
12	3.762	827	831	833	rBV	388	258	0.03%	0.004%
13	3.885	867	869	875	rBV2	395	231	0.03%	0.003%
14	3.939	875	886	915	rBV	54829	165805	18.55%	2.414%
15	4.897	1182	1184	1185	rVB	359	91	0.01%	0.001%
16	4.920	1189	1191	1194	rBV2	299	178	0.02%	0.003%
17	4.974	1205	1208	1211	rBV2	426	298	0.03%	0.004%
18	5.093	1228	1245	1272	rBV2	352844	893702	100.00%	13.012%
19	5.659	1410	1421	1450	rVB	304838	597131	66.82%	8.694%
20	5.958	1501	1514	1536	rBV	193481	374802	41.94%	5.457%
21	6.113	1549	1562	1589	rBV	197830	402902	45.08%	5.866%
22	6.315	1622	1625	1626	rBV	418	177	0.02%	0.003%
23	6.409	1650	1654	1656	rBV2	663	455	0.05%	0.007%
24	6.482	1676	1677	1680	rBV	564	193	0.02%	0.003%
25	6.585	1707	1709	1712	rBV	242	66	0.01%	0.001%
26	6.601	1712	1714	1716	rBV	391	180	0.02%	0.003%
27	6.762	1762	1764	1765	rBV	314	116	0.01%	0.002%
28	6.794	1771	1774	1777	rVB2	492	310	0.03%	0.005%
29	6.817	1777	1781	1786	rBV3	353	300	0.03%	0.004%
30	6.917	1810	1812	1813	rBV	452	173	0.02%	0.003%
31	7.026	1835	1846	1867	rBV2	121289	212471	23.77%	3.094%
32	7.277	1922	1924	1925	rBV	254	75	0.01%	0.001%
33	7.357	1934	1949	1975	rBV	439097	767549	85.88%	11.176%
34	7.659	2029	2043	2058	rBV	85709	144684	16.19%	2.107%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022020\
 Data File : VV014636.D
 Acq On : 20 Feb 2020 20:07
 Operator : SY/MD
 Sample : L1607-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis

35	7.888	2112	2114	2117	rBV2	272	187	0.02%	0.003%
36	8.003	2149	2150	2151	rVB2	403	78	0.01%	0.001%
37	8.080	2172	2174	2176	rBV3	366	185	0.02%	0.003%
38	8.132	2179	2190	2227	rBV	197915	374336	41.89%	5.450%
39	8.598	2333	2335	2336	rBV	291	102	0.01%	0.001%
40	8.640	2345	2348	2349	rVB	386	125	0.01%	0.002%
41	8.656	2351	2353	2355	rVV	407	126	0.01%	0.002%
42	8.691	2361	2364	2366	rBV2	323	167	0.02%	0.002%
43	8.727	2374	2375	2376	rBV2	112	30	0.00%	0.000%
44	8.891	2413	2426	2443	rBV	448585	726637	81.31%	10.580%
45	9.177	2513	2515	2517	rBV2	389	199	0.02%	0.003%
46	9.283	2545	2548	2550	rBV2	399	219	0.02%	0.003%
47	9.315	2555	2558	2566	rVV	4510	2983	0.33%	0.043%
48	9.351	2566	2569	2574	rVB2	356	281	0.03%	0.004%
49	9.441	2595	2597	2600	rBV	425	203	0.02%	0.003%
50	9.621	2646	2653	2654	rBV	363	316	0.04%	0.005%
51	9.797	2705	2708	2709	rBV2	432	230	0.03%	0.003%
52	10.000	2770	2771	2772	rBV2	303	99	0.01%	0.001%
53	10.187	2827	2829	2830	rBV2	563	185	0.02%	0.003%
54	10.254	2838	2850	2872	rBV	269875	421272	47.14%	6.134%
55	10.437	2906	2907	2908	rBV	247	65	0.01%	0.001%
56	10.537	2937	2938	2940	rVB	542	162	0.02%	0.002%
57	10.585	2951	2953	2955	rBV2	437	149	0.02%	0.002%
58	10.611	2959	2961	2964	rBV2	413	200	0.02%	0.003%
59	10.813	3023	3024	3026	rBV	419	148	0.02%	0.002%
60	10.923	3052	3058	3059	rBV2	395	341	0.04%	0.005%
61	10.949	3063	3066	3068	rBV	549	321	0.04%	0.005%
62	11.203	3142	3145	3147	rBV	414	255	0.03%	0.004%
63	11.289	3160	3172	3193	rBV	456769	719494	80.51%	10.476%
64	11.666	3278	3289	3309	rBV	442528	693546	77.60%	10.098%
65	12.032	3398	3403	3405	rBV2	359	242	0.03%	0.004%
66	12.270	3476	3477	3479	rBV	325	120	0.01%	0.002%
67	12.984	3698	3699	3703	rVB2	428	204	0.02%	0.003%
68	13.038	3713	3716	3718	rBV2	373	194	0.02%	0.003%


Sum of corrected areas: 6868100

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022020\
Data File : VV014636.D
Acq On : 20 Feb 2020 20:07
Operator : SY/MD
Sample : L1607-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

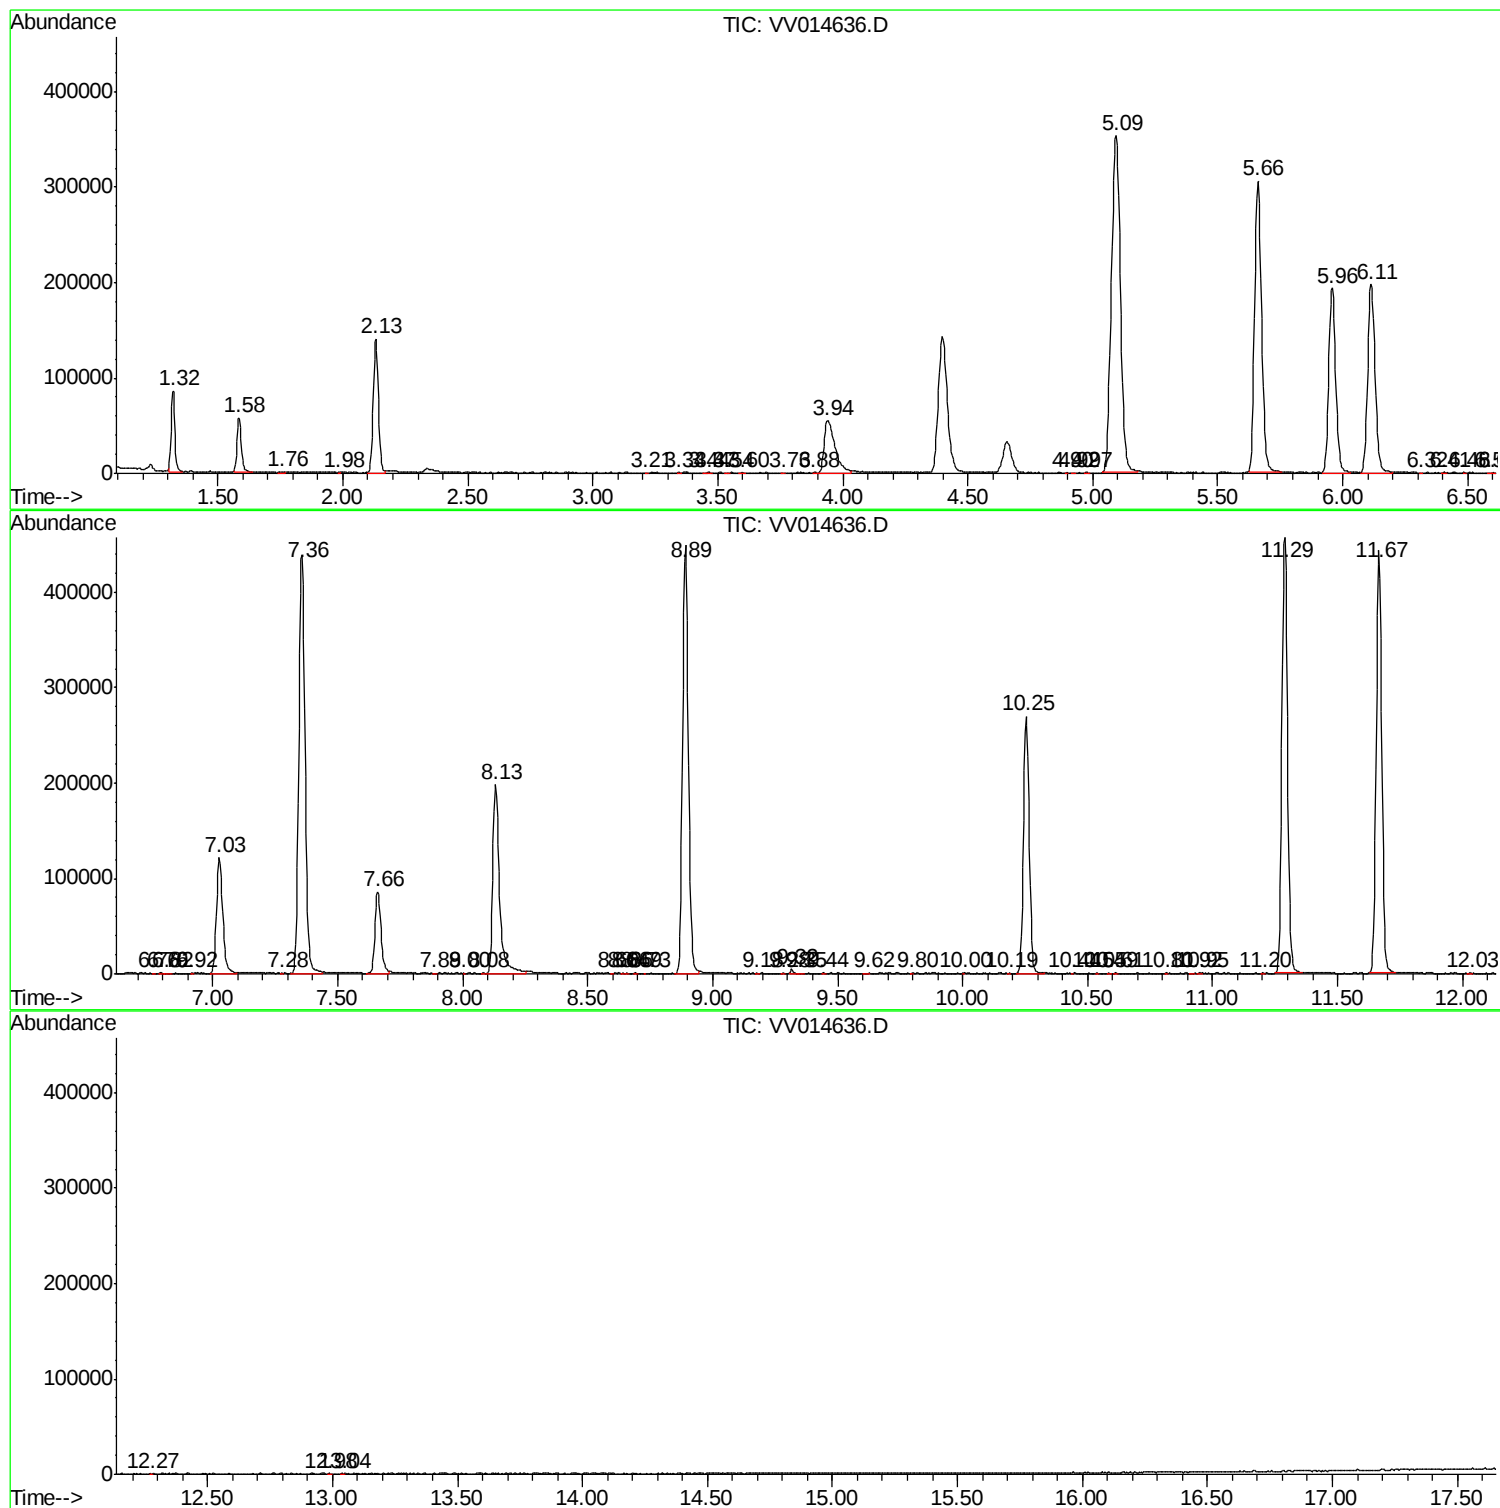

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014636.D
Acq On : 20 Feb 2020 20:07
Operator : SY/MD
Sample : L1607-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022020\
Data File : VV014636.D
Acq On : 20 Feb 2020 20:07
Operator : SY/MD
Sample : L1607-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc