


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV022020\
 Data File : VV014617.D
 Acq On : 20 Feb 2020 11:30
 Operator : SY/MD
 Sample : BFB93
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB93

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM021220WMA.M
 Title : VOC Analysis
 Last Update : Mon Feb 24 17:23:09 2020

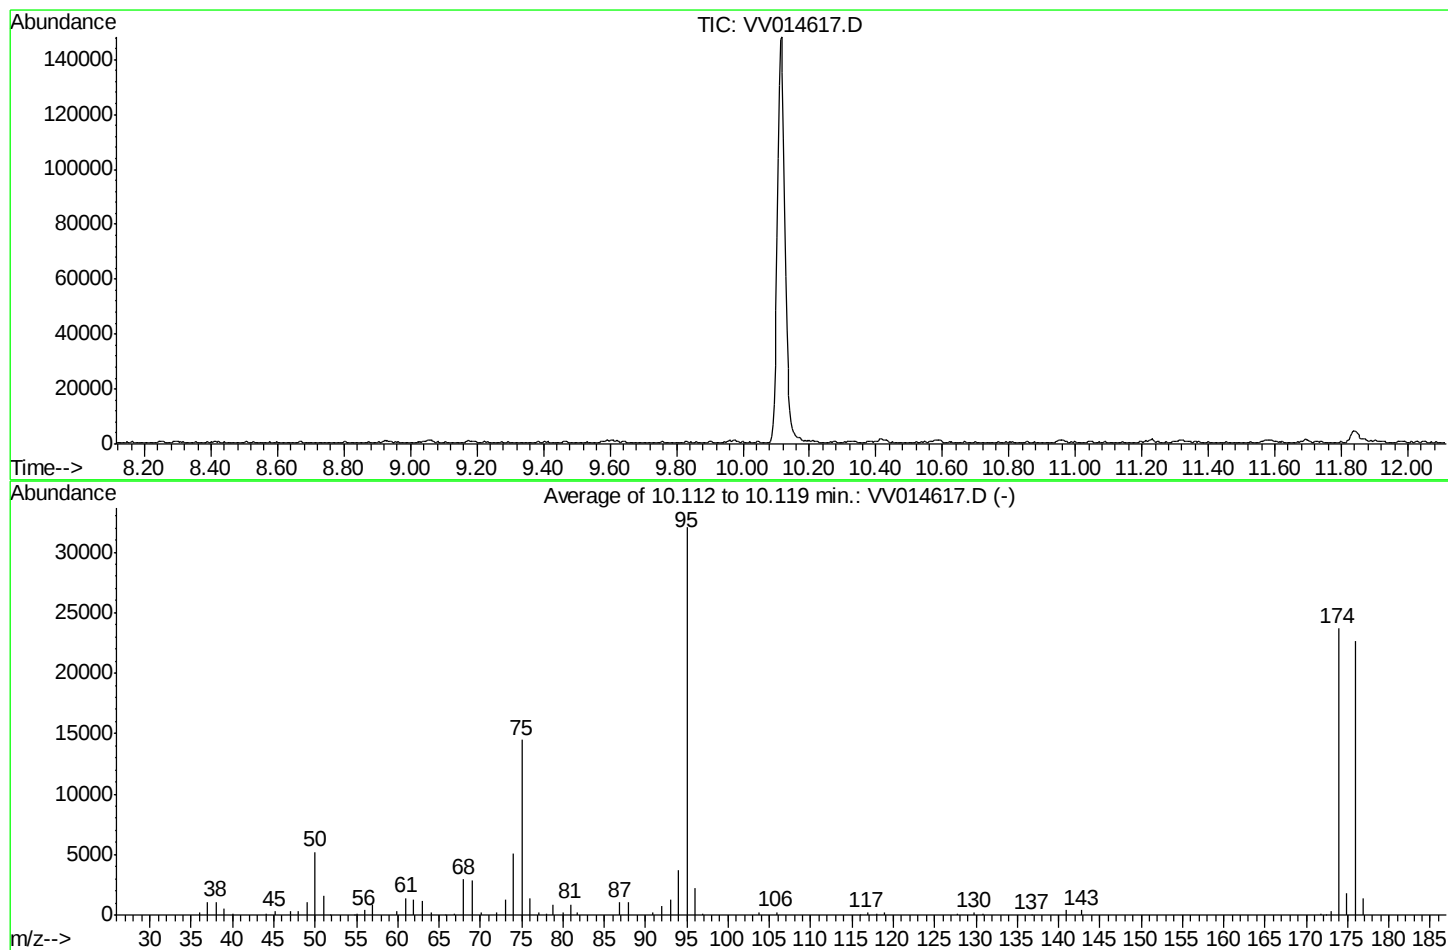

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	5212	PASS
75	95	30	80	45.1	14452	PASS
95	95	100	100	100.0	32053	PASS
96	95	5	9	6.8	2184	PASS
173	174	0.00	2	1.5	362	PASS
174	95	50	120	74.0	23704	PASS
175	174	5	9	7.4	1757	PASS
176	174	95	101	95.4	22616	PASS
177	176	5	9	6.3	1431	PASS

m/z	Abundance
35.90	219.0
36.90	1232.0
38.00	1072.0
39.00	565.0
40.00	266.0
44.00	427.0
45.10	266.0
47.00	265.0
47.90	290.0
49.00	1011.0
50.00	5476.0
51.00	1694.0
51.90	125.0
54.80	173.0
55.90	445.0
57.00	846.0
59.90	329.0
61.00	1435.0
61.90	1306.0
63.00	1198.0
64.00	183.0
65.70	106.0
66.90	137.0
68.00	3084.0
69.00	2850.0
70.20	238.0
72.00	241.0
73.00	1433.0
74.00	5230.0
75.00	14888.0
76.00	1528.0
77.00	226.0
78.00	176.0
78.80	823.0
79.90	264.0
80.90	897.0
81.80	220.0
86.90	1133.0
88.00	1068.0
90.90	211.0
91.90	786.0
93.00	1301.0
94.00	3838.0
95.00	32832.0
96.00	2248.0
96.90	116.0
103.80	206.0
105.90	250.0
116.90	159.0
118.00	178.0
118.90	195.0
127.80	128.0
129.80	204.0
130.80	122.0
140.90	456.0
142.90	353.0
171.70	111.0
172.40	151.0
173.00	368.0
173.90	23864.0
174.90	1754.0
175.90	22720.0
176.90	1424.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

m/z	Abundance
36.00	255.0
36.90	1034.0
38.00	1120.0
39.00	500.0
40.00	228.0
44.00	413.0
45.10	322.0
47.00	296.0
47.90	295.0
49.00	1124.0
50.00	5380.0
51.00	1627.0
55.00	187.0
56.00	393.0
57.00	826.0
59.90	332.0
61.00	1478.0
62.00	1285.0
63.00	1184.0
64.00	195.0
66.90	125.0
68.00	3003.0
69.00	2937.0
70.10	210.0
72.00	199.0
73.00	1364.0
74.00	5287.0
75.00	14929.0
76.00	1359.0
77.00	200.0
78.00	164.0
78.80	838.0
80.00	245.0
80.90	922.0
81.80	238.0
86.90	1080.0
88.00	1042.0
90.90	191.0
91.90	780.0
93.00	1263.0
94.00	3786.0
95.00	33208.0
96.00	2280.0
96.90	108.0
103.80	189.0
105.90	213.0
116.90	167.0
118.00	163.0
119.00	171.0
127.80	156.0
129.80	171.0
130.80	153.0
140.90	377.0
142.90	419.0
171.80	121.0
173.00	394.0
173.90	24592.0
174.90	1835.0
175.90	23384.0
176.90	1497.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

m/z	Abundance
36.00	262.0
36.90	852.0
38.00	1059.0
39.00	399.0
40.00	211.0
44.00	384.0
45.10	338.0
46.90	306.0
47.90	258.0
49.00	1158.0
50.00	4782.0
51.00	1365.0
55.00	171.0
56.00	383.0
57.00	739.0
59.90	337.0
61.00	1363.0
62.00	1268.0
63.00	986.0
64.00	164.0
68.00	2733.0
69.00	2890.0
70.00	189.0
72.00	193.0
73.00	1135.0
74.00	4607.0
75.00	13539.0
76.00	1115.0
77.10	168.0
77.90	115.0
78.90	822.0
79.90	208.0
80.90	841.0
81.80	223.0
86.90	875.0
88.00	960.0
90.90	141.0
91.90	698.0
93.00	1171.0
94.00	3344.0
95.00	30120.0
96.00	2026.0
103.80	170.0
105.80	186.0
115.90	117.0
116.80	199.0
118.00	110.0
119.00	141.0
127.80	136.0
129.80	139.0
130.80	136.0
136.80	103.0
140.90	344.0
142.80	430.0
171.70	128.0
173.00	325.0
173.90	22656.0
174.90	1683.0
175.90	21744.0
177.00	1372.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

Scan 2794 (10.074 min): VV014617.D
BFB93

m/z	Abundance
36.30	104.0
40.00	142.0
44.00	295.0
52.40	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93