

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022023\
 Data File : VV030071.D
 Acq On : 20 Feb 2023 10:49
 Operator : SY/MD
 Sample : VV0220MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK316

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.221	52	56	62	rBV	7525	8043	0.65%	0.079%
2	1.282	69	75	93	rVB	140304	154770	12.57%	1.520%
3	1.536	147	154	173	rVB	127592	156006	12.67%	1.532%
4	2.066	309	319	333	rBV	254712	369964	30.06%	3.633%
5	2.243	367	374	375	rBV6	1451	1386	0.11%	0.014%
6	2.359	407	410	411	rBV	302	175	0.01%	0.002%
7	2.388	416	419	423	rVB4	632	494	0.04%	0.005%
8	2.452	433	439	448	rBV3	2348	3493	0.28%	0.034%
9	2.510	454	457	461	rBV2	306	220	0.02%	0.002%
10	2.597	481	484	486	rBV3	341	277	0.02%	0.003%
11	2.616	488	490	494	rVB3	258	184	0.01%	0.002%
12	2.709	513	519	523	rVB5	630	638	0.05%	0.006%
13	2.777	537	540	543	rBV	279	209	0.02%	0.002%
14	2.831	550	557	563	rBV2	179	297	0.02%	0.003%
15	3.494	757	763	765	rBV	258	225	0.02%	0.002%
16	3.645	805	810	813	rBV	303	296	0.02%	0.003%
17	3.799	846	858	902	rBV	101048	291985	23.72%	2.867%
18	4.262	983	1002	1032	rBV	191331	488583	39.69%	4.798%
19	4.609	1107	1110	1114	rVB3	343	248	0.02%	0.002%
20	4.796	1164	1168	1171	rBV2	292	252	0.02%	0.002%
21	4.966	1203	1221	1250	rBV2	439128	1173996	95.38%	11.528%
22	5.243	1304	1307	1312	rBV4	418	421	0.03%	0.004%
23	5.394	1351	1354	1358	rVV2	243	267	0.02%	0.003%
24	5.420	1358	1362	1366	rVB2	481	387	0.03%	0.004%
25	5.542	1383	1400	1423	rBV	432059	884948	71.90%	8.690%
26	5.777	1470	1473	1476	rBV	388	287	0.02%	0.003%
27	5.828	1484	1489	1491	rBV3	1177	1111	0.09%	0.011%
28	5.998	1526	1542	1565	rBV	263887	545727	44.34%	5.359%
29	6.307	1636	1638	1643	rVB2	274	187	0.02%	0.002%
30	6.381	1658	1661	1662	rVV	269	162	0.01%	0.002%
31	6.478	1687	1691	1694	rVV3	244	214	0.02%	0.002%
32	6.564	1710	1718	1725	rBV4	598	1087	0.09%	0.011%
33	6.629	1734	1738	1739	rBV2	260	177	0.01%	0.002%
34	6.638	1739	1741	1746	rVB	257	176	0.01%	0.002%
35	6.699	1756	1760	1766	rVB2	247	243	0.02%	0.002%
36	6.921	1816	1829	1847	rBV	152972	275770	22.40%	2.708%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022023\
 Data File : VV030071.D
 Acq On : 20 Feb 2023 10:49
 Operator : SY/MD
 Sample : VV0220MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK316

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
 Title : VOC Analysis

37	7.175	1905	1908	1909	rBV2	352	211	0.02%	0.002%
38	7.198	1913	1915	1919	rVB	237	174	0.01%	0.002%
39	7.252	1919	1932	1955	rBV	542402	943979	76.69%	9.270%
40	7.516	2010	2014	2016	rBV3	295	219	0.02%	0.002%
41	7.561	2016	2028	2052	rBV	104494	185459	15.07%	1.821%
42	7.773	2089	2094	2096	rBV3	379	259	0.02%	0.003%
43	7.793	2096	2100	2102	rVB2	287	170	0.01%	0.002%
44	7.879	2120	2127	2129	rBV3	564	598	0.05%	0.006%
45	7.969	2151	2155	2160	rVB3	277	259	0.02%	0.003%
46	8.034	2163	2175	2208	rBV	353917	618326	50.24%	6.072%
47	8.236	2235	2238	2240	rVB3	503	255	0.02%	0.003%
48	8.368	2269	2279	2291	rBV3	4329	7633	0.62%	0.075%
49	8.490	2312	2317	2322	rBV	292	263	0.02%	0.003%
50	8.590	2344	2348	2351	rBV	415	304	0.02%	0.003%
51	8.693	2375	2380	2383	rBV2	203	180	0.01%	0.002%
52	8.722	2386	2389	2395	rVB	193	172	0.01%	0.002%
53	8.793	2398	2411	2450	rBV	674199	1088599	88.44%	10.690%
54	8.960	2456	2463	2472	rBV5	822	1421	0.12%	0.014%
55	9.082	2497	2501	2503	rBV2	634	490	0.04%	0.005%
56	9.487	2623	2627	2629	rBV2	479	367	0.03%	0.004%
57	9.513	2629	2635	2641	rVV5	1275	1726	0.14%	0.017%
58	9.555	2645	2648	2650	rBV2	238	169	0.01%	0.002%
59	9.702	2691	2694	2698	rBV2	344	174	0.01%	0.002%
60	9.770	2712	2715	2722	rVB3	363	359	0.03%	0.004%
61	9.866	2742	2745	2749	rBV2	548	539	0.04%	0.005%
62	10.014	2789	2791	2795	rVB	277	189	0.02%	0.002%
63	10.056	2802	2804	2810	rVB2	211	184	0.01%	0.002%
64	10.162	2823	2837	2858	rBV	440660	699822	56.86%	6.872%
65	10.407	2910	2913	2917	rBV	184	180	0.01%	0.002%
66	10.484	2934	2937	2942	rVB2	408	441	0.04%	0.004%
67	10.628	2979	2982	2987	rBV2	283	192	0.02%	0.002%
68	10.686	2997	3000	3004	rVB2	313	246	0.02%	0.002%
69	10.818	3039	3041	3045	rVB	332	203	0.02%	0.002%
70	10.863	3049	3055	3061	rBV4	970	1277	0.10%	0.013%
71	10.950	3080	3082	3089	rVB2	292	259	0.02%	0.003%
72	10.992	3089	3095	3099	rBV	277	407	0.03%	0.004%
73	11.130	3132	3138	3145	rVB3	1451	1789	0.15%	0.018%
74	11.194	3145	3158	3181	rBV	802198	1230857	100.00%	12.087%
75	11.352	3205	3207	3209	rVB	422	173	0.01%	0.002%
76	11.403	3221	3223	3226	rBV	273	164	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022023\
 Data File : VV030071.D
 Acq On : 20 Feb 2023 10:49
 Operator : SY/MD
 Sample : VV0220MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK316

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
 Title : VOC Analysis

77	11.477	3242	3246	3249	rBV2	261	193	0.02%	0.002%
78	11.571	3263	3275	3291	rBV	638616	1002610	81.46%	9.845%
79	11.680	3307	3309	3312	rBV3	675	413	0.03%	0.004%
80	11.760	3328	3334	3335	rBV4	951	823	0.07%	0.008%
81	11.918	3380	3383	3388	rBV	216	208	0.02%	0.002%
82	12.011	3410	3412	3414	rBV3	300	165	0.01%	0.002%
83	12.153	3453	3456	3460	rVV2	359	290	0.02%	0.003%
84	12.201	3466	3471	3473	rBV3	995	888	0.07%	0.009%
85	12.593	3586	3593	3605	rVB6	1946	2912	0.24%	0.029%
86	12.689	3621	3623	3629	rVB3	300	319	0.03%	0.003%
87	12.722	3629	3633	3635	rBV	365	318	0.03%	0.003%
88	12.792	3651	3655	3656	rBV2	444	257	0.02%	0.003%
89	12.841	3668	3670	3674	rVV3	318	190	0.02%	0.002%
90	13.027	3725	3728	3732	rBV2	297	262	0.02%	0.003%
91	13.079	3741	3744	3749	rBV3	321	261	0.02%	0.003%
92	13.210	3779	3785	3793	rVB4	3114	4313	0.35%	0.042%
93	13.452	3852	3860	3870	rBV2	4854	7189	0.58%	0.071%
94	13.548	3887	3890	3893	rBV3	415	312	0.03%	0.003%
95	13.693	3927	3935	3947	rVB4	3230	4784	0.39%	0.047%
96	13.760	3954	3956	3958	rBV	444	215	0.02%	0.002%
97	13.927	4004	4008	4009	rBV2	398	270	0.02%	0.003%
98	13.998	4022	4030	4037	rVB3	2567	3638	0.30%	0.036%
99	14.030	4037	4040	4045	rVB3	386	229	0.02%	0.002%
100	14.394	4149	4153	4157	rBV5	830	933	0.08%	0.009%




Sum of corrected areas: 10183585

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022023\
Data File : VV030071.D
Acq On : 20 Feb 2023 10:49
Operator : SY/MD
Sample : VV0220MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

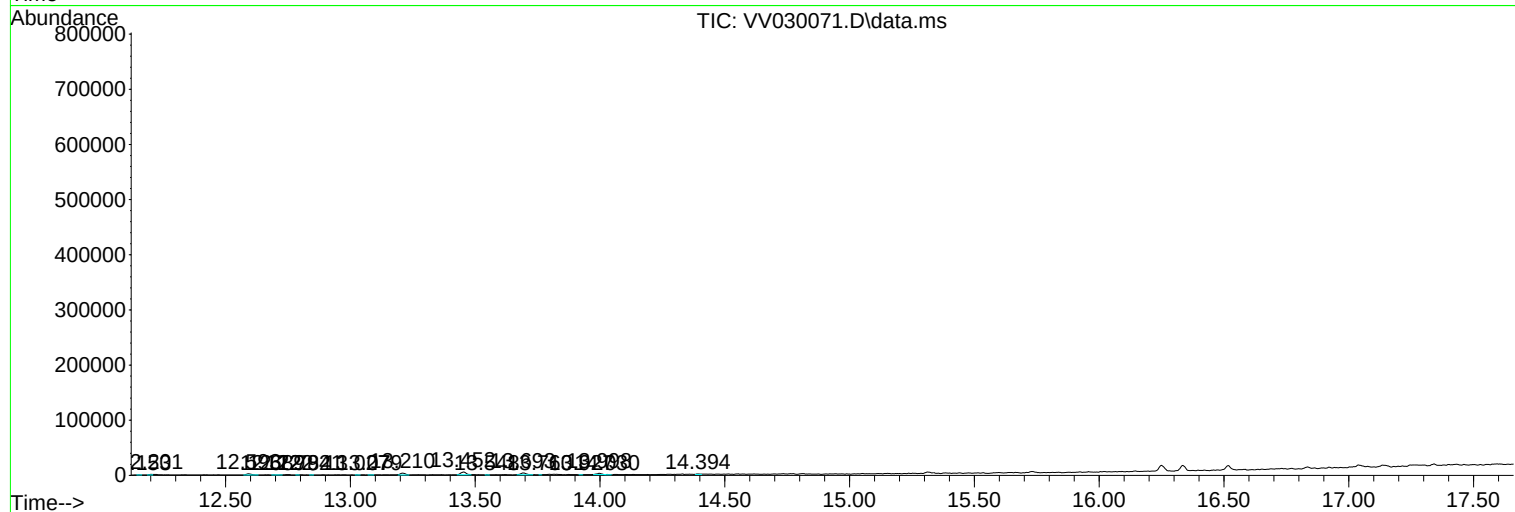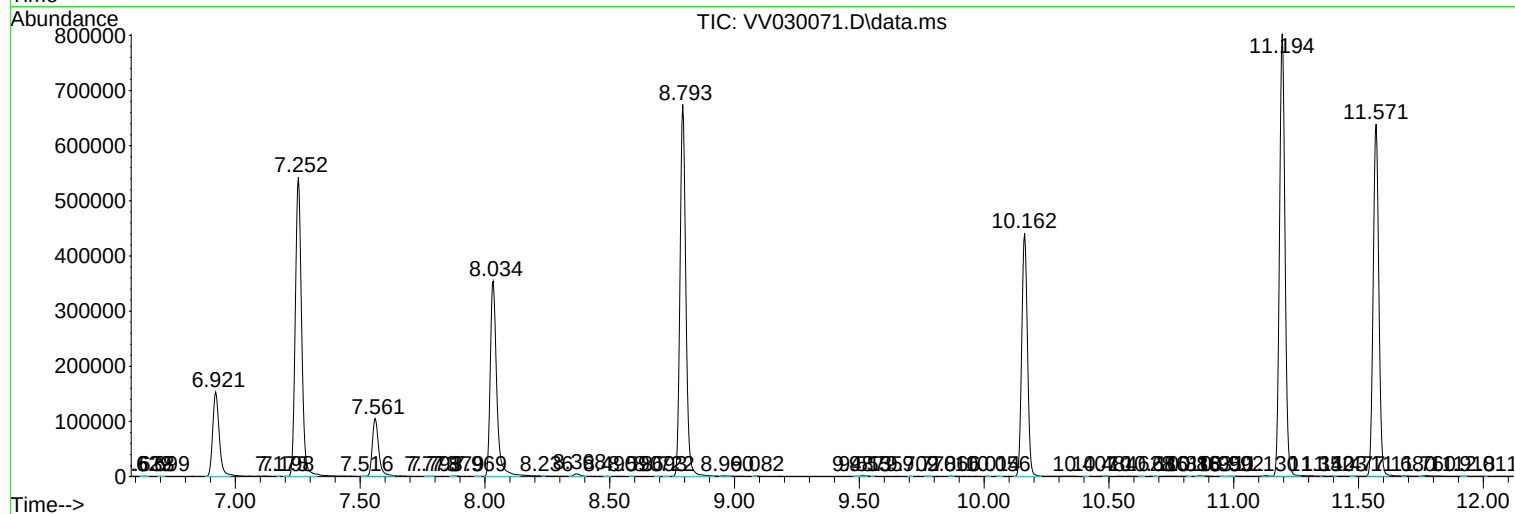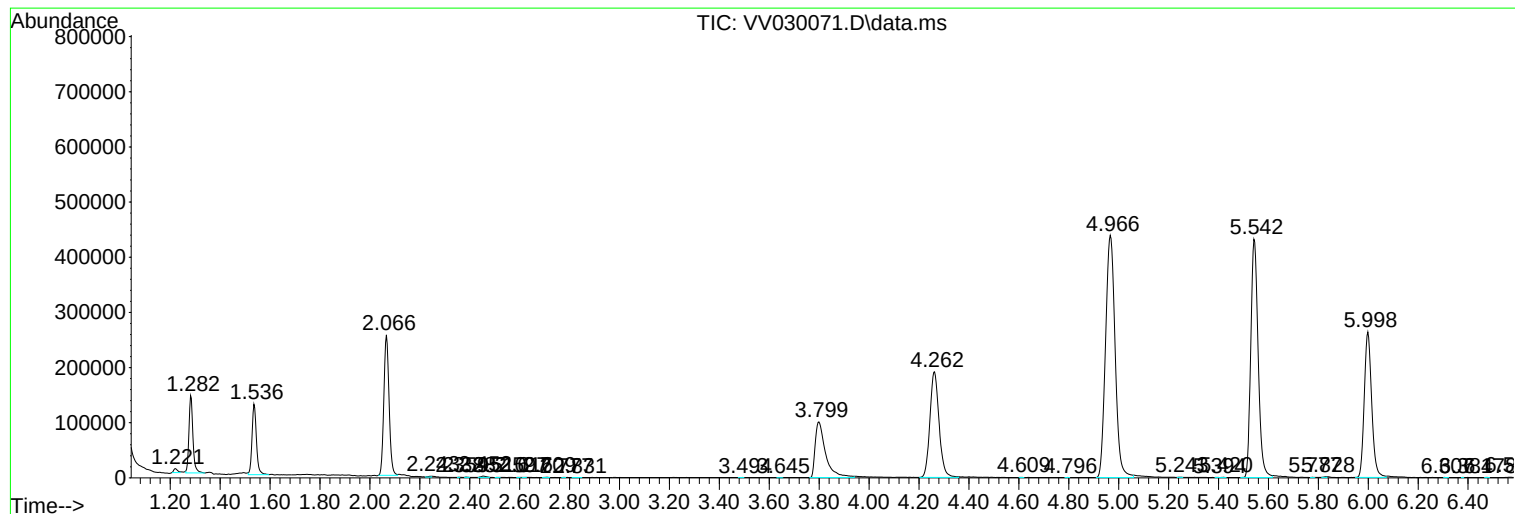

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022023\
Data File : VV030071.D
Acq On : 20 Feb 2023 10:49
Operator : SY/MD
Sample : VV0220MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022023\
Data File : VV030071.D
Acq On : 20 Feb 2023 10:49
Operator : SY/MD
Sample : VV0220MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc