


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022023\
Data File : VV030069.D
Acq On : 20 Feb 2023 08:40
Operator : SY/MD
Sample : BFB364
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB364

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
Title : VOC Analysis
Last Update : Mon Feb 20 22:59:49 2023

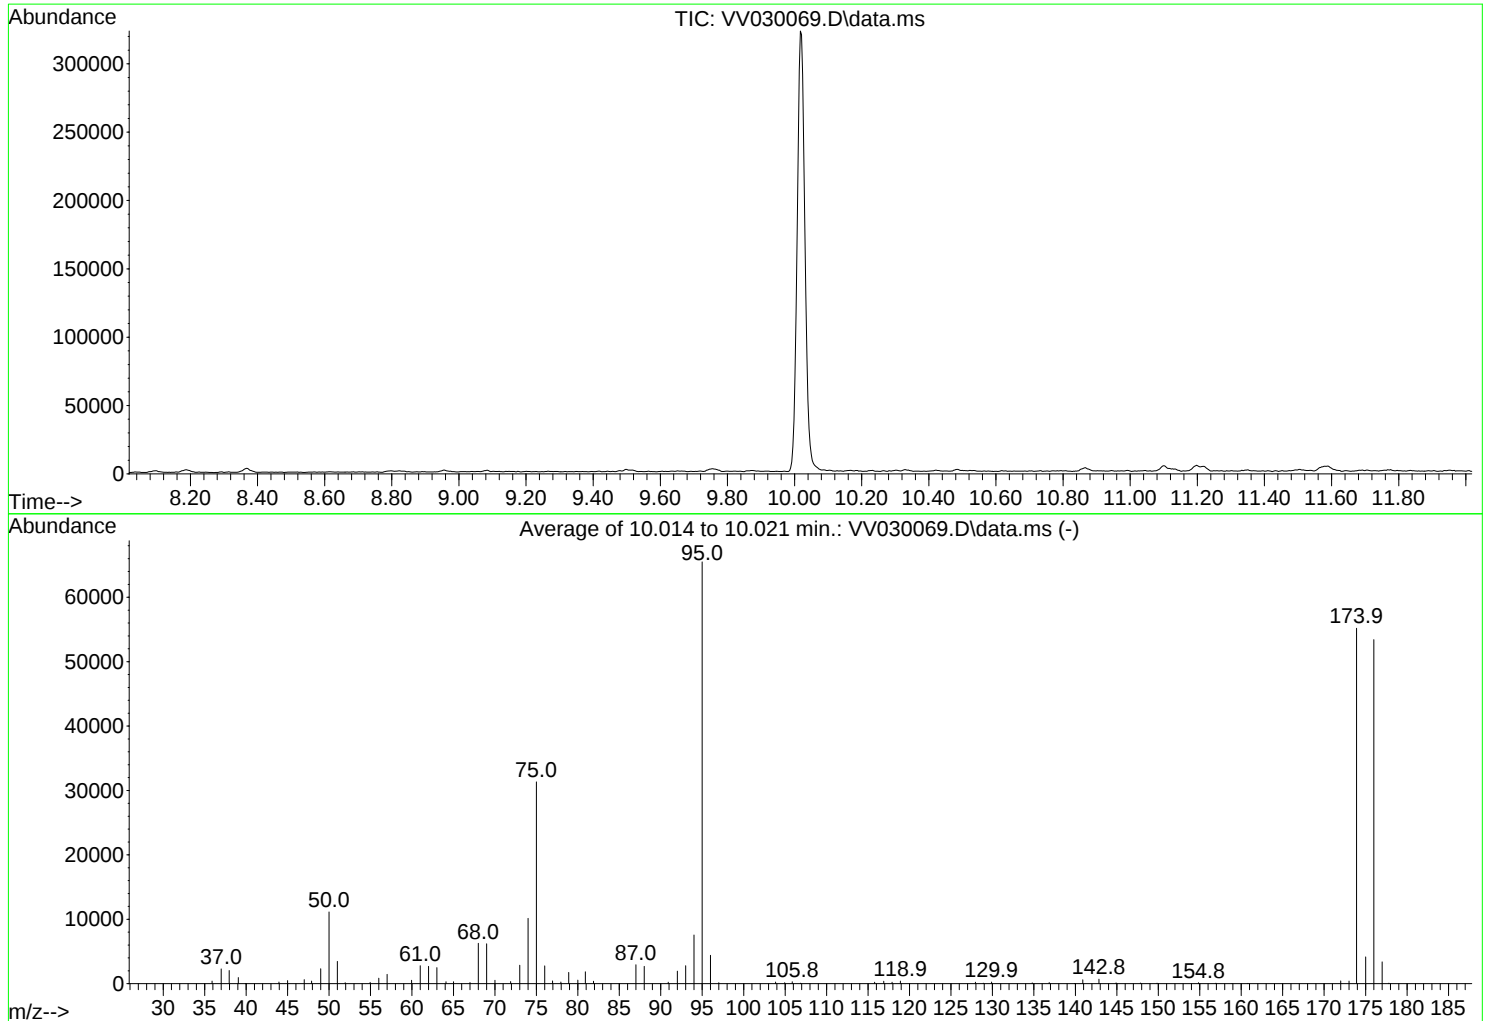

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	11137	PASS
75	95	30	80	47.8	31333	PASS
95	95	100	100	100.0	65507	PASS
96	95	5	9	6.7	4397	PASS
173	174	0.00	2	0.7	410	PASS
174	95	50	120	84.3	55192	PASS
175	174	5	9	7.5	4154	PASS
176	174	95	105	96.8	53419	PASS
177	176	5	10	6.4	3395	PASS

m/z	Abundance
35.90	812.0
37.90	302.0
39.90	154.0
43.90	464.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

m/z	Abundance
36.00	1301.0
37.00	2309.0
38.00	2286.0
39.10	870.0
40.00	157.0
44.00	706.0
45.00	447.0
47.00	628.0
47.90	407.0
49.00	2296.0
50.00	10867.0
51.00	3276.0
51.90	177.0
55.00	178.0
56.00	829.0
57.00	1370.0
59.90	490.0
61.00	2673.0
62.00	2610.0
63.00	2328.0
64.10	331.0
65.00	258.0
67.00	176.0
68.00	5964.0
69.00	6041.0
70.00	462.0
71.80	329.0
73.00	2509.0
74.00	9864.0
75.00	29480.0
76.00	2644.0
76.90	423.0
78.00	279.0
78.90	1602.0
80.00	541.0
80.90	1825.0
81.90	351.0
87.00	2709.0
88.00	2576.0
90.90	218.0
92.00	1842.0
93.00	2670.0
94.00	7155.0
95.00	61824.0
96.00	4279.0
97.00	135.0
103.90	255.0
105.00	143.0
105.80	314.0
115.80	217.0
116.90	364.0
117.90	207.0
118.90	368.0
127.90	261.0
128.90	110.0
129.90	228.0
134.80	125.0
136.80	147.0
140.90	475.0
142.80	643.0
144.90	140.0
149.80	105.0
154.90	163.0
157.00	138.0
158.90	101.0
172.00	429.0
173.00	587.0
173.90	50968.0
175.00	3702.0
176.00	49160.0
177.00	3318.0
177.80	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

m/z	Abundance
36.00	1218.0
37.00	2367.0
38.00	2386.0
39.10	994.0
39.90	162.0
44.00	728.0
45.00	478.0
47.00	633.0
47.90	418.0
49.00	2394.0
50.00	11564.0
51.00	3611.0
51.90	171.0
55.00	196.0
56.00	872.0
57.00	1500.0
60.00	536.0
61.00	2880.0
62.00	2802.0
63.00	2569.0
64.10	306.0
65.00	298.0
67.00	162.0
68.00	6463.0
69.00	6403.0
70.00	544.0
71.90	318.0
73.00	2977.0
74.00	10440.0
75.00	32280.0
76.00	2847.0
76.90	441.0
77.90	243.0
78.90	1849.0
80.00	573.0
80.90	1867.0
81.90	375.0
87.00	2999.0
88.00	2818.0
90.90	230.0
92.00	2039.0
93.00	2861.0
94.00	7784.0
95.00	67624.0
96.00	4527.0
97.00	148.0
103.80	256.0
104.90	168.0
105.80	314.0
106.80	104.0
115.80	243.0
116.90	396.0
117.90	222.0
118.90	437.0
127.90	236.0
128.90	116.0
129.90	272.0
134.80	131.0
136.80	183.0
140.90	609.0
142.90	733.0
144.90	138.0
147.90	119.0
149.90	102.0
154.90	167.0
156.90	111.0
172.00	422.0
173.00	643.0
173.90	56928.0
175.00	4327.0
176.00	55152.0
177.00	3469.0
177.80	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

m/z	Abundance
36.00	1137.0
37.00	2178.0
38.00	2370.0
39.00	986.0
39.90	185.0
44.00	689.0
45.00	494.0
47.00	591.0
47.90	346.0
49.00	2219.0
50.00	10981.0
51.00	3468.0
52.00	142.0
54.90	201.0
56.00	817.0
57.00	1450.0
60.00	517.0
61.00	2808.0
62.00	2637.0
63.00	2539.0
64.10	251.0
65.00	325.0
67.00	182.0
68.00	6347.0
69.00	6166.0
70.00	544.0
72.00	316.0
73.00	3106.0
74.00	10124.0
75.00	32240.0
76.00	2752.0
77.00	384.0
77.90	204.0
78.90	1814.0
80.00	541.0
80.90	1822.0
81.90	399.0
87.00	3081.0
88.00	2678.0
90.90	248.0
92.00	1949.0
93.00	2785.0
94.00	7739.0
95.00	67072.0
96.00	4386.0
97.00	176.0
103.80	261.0
104.90	167.0
105.90	282.0
106.90	131.0
115.80	231.0
116.90	400.0
117.90	226.0
118.90	423.0
128.00	193.0
129.90	282.0
134.80	122.0
136.90	188.0
139.90	113.0
140.90	696.0
142.90	735.0
144.90	136.0
147.80	166.0
154.80	160.0
160.80	141.0
172.00	405.0
173.90	57680.0
175.00	4432.0
176.00	55944.0
177.00	3397.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364