


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022119\
 Data File : VV009314.D
 Acq On : 21 Feb 2019 09:07
 Operator : SY/MD
 Sample : BFB64
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB64

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM022019S.M
 Title : VOC Analysis
 Last Update : Tue Feb 26 02:46:42 2019

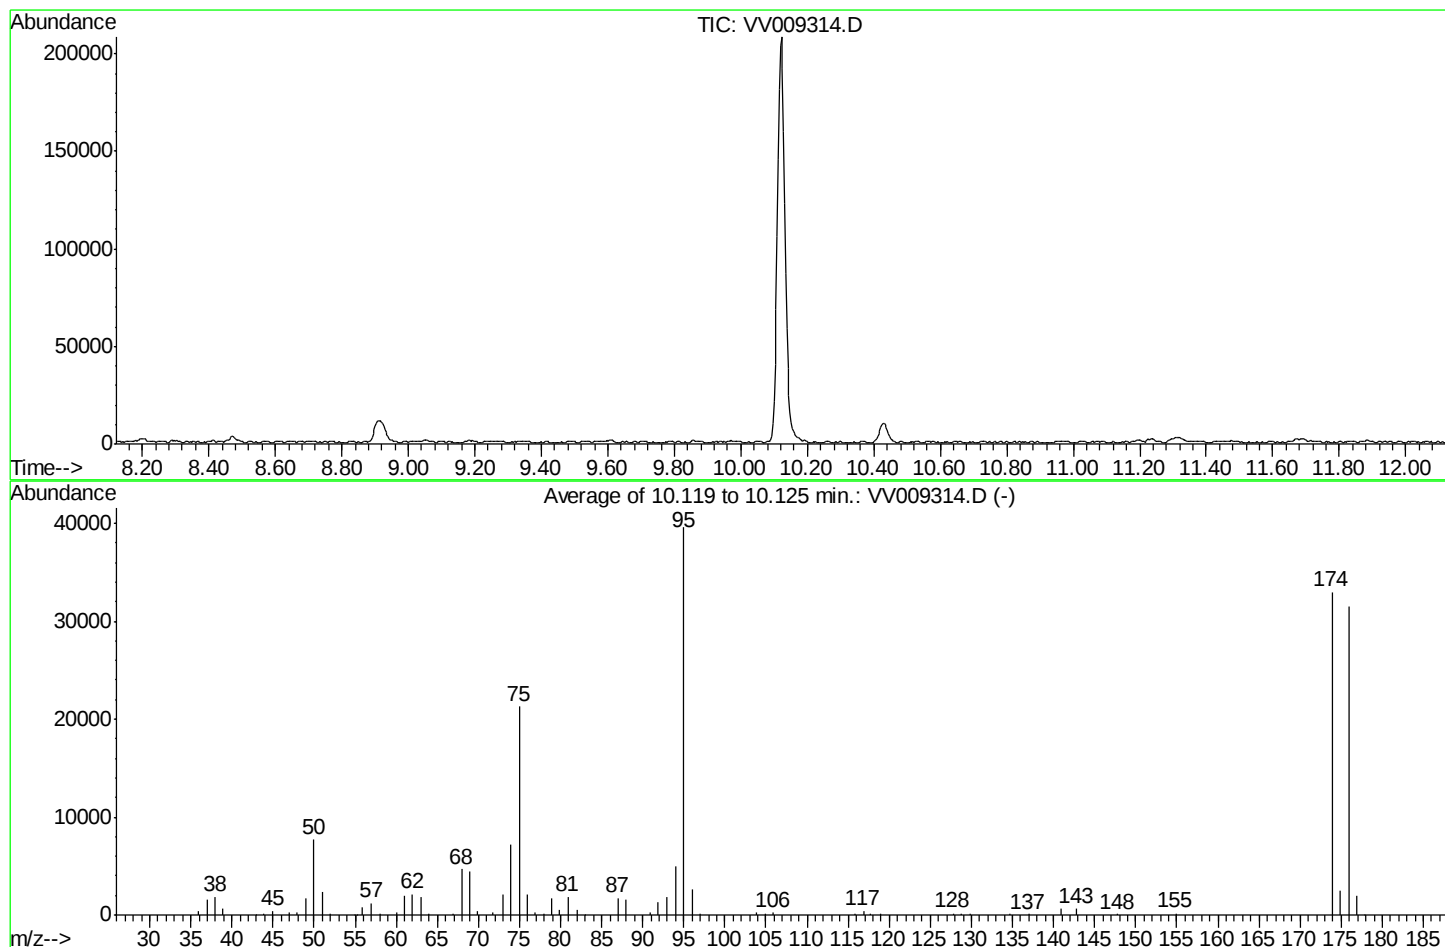

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	7682	PASS
75	95	30	80	53.8	21304	PASS
95	95	100	100	100.0	39602	PASS
96	95	5	9	6.6	2598	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.3	32997	PASS
175	174	5	9	7.6	2508	PASS
176	174	95	101	95.6	31557	PASS
177	176	5	9	6.3	1982	PASS

m/z	Abundance
36.00	467.0
37.00	1722.0
38.00	1973.0
39.00	785.0
40.00	133.0
41.00	170.0
43.00	198.0
43.90	526.0
45.00	434.0
47.00	305.0
47.80	223.0
49.00	1900.0
50.00	7784.0
51.00	2461.0
51.90	165.0
55.00	204.0
55.90	791.0
57.00	1343.0
60.00	295.0
61.00	2125.0
62.00	2037.0
63.00	1861.0
63.90	180.0
66.90	207.0
68.00	4738.0
69.00	4717.0
70.00	398.0
71.80	245.0
73.00	2135.0
74.00	7177.0
75.00	21984.0
76.00	2144.0
76.90	289.0
78.00	159.0
78.90	1878.0
79.80	575.0
80.90	1836.0
81.90	450.0
82.90	104.0
87.00	1853.0
87.90	1565.0
90.90	223.0
91.90	1401.0
92.90	1707.0
94.00	4925.0
95.00	40272.0
96.00	2614.0
103.90	254.0
104.90	128.0
105.90	249.0
115.80	202.0
116.80	378.0
117.70	167.0
118.90	216.0
127.80	160.0
128.70	108.0
129.80	147.0
137.00	112.0
140.90	589.0
142.80	634.0
154.90	159.0
173.90	32776.0
174.90	2623.0
175.90	31176.0
176.90	2015.0
177.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	446.0
37.00	1628.0
38.00	1948.0
39.00	740.0
40.00	121.0
41.10	166.0
43.00	173.0
44.00	581.0
45.00	475.0
47.00	324.0
47.90	218.0
49.00	1784.0
50.00	8007.0
51.00	2442.0
52.00	157.0
54.90	211.0
55.20	198.0
55.90	851.0
57.00	1365.0
58.00	104.0
60.00	264.0
61.10	1987.0
62.00	2242.0
63.00	1854.0
63.90	151.0
66.80	205.0
68.00	4863.0
69.00	4572.0
69.90	408.0
71.80	231.0
73.00	2143.0
74.00	7509.0
75.00	21944.0
76.00	2127.0
76.90	289.0
77.90	123.0
78.90	1749.0
79.90	572.0
80.90	1935.0
82.00	492.0
83.00	103.0
86.90	1805.0
87.90	1684.0
90.80	240.0
91.90	1398.0
92.90	1851.0
94.00	4996.0
95.00	40992.0
96.00	2649.0
97.00	133.0
103.90	231.0
105.00	120.0
105.90	254.0
115.80	200.0
116.90	419.0
117.70	172.0
118.90	182.0
127.80	181.0
128.70	115.0
129.80	158.0
134.70	118.0
136.90	109.0
140.90	638.0
142.80	659.0
147.80	127.0
154.90	158.0
173.90	34008.0
174.90	2556.0
175.90	32824.0
176.90	2004.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.90	367.0
36.90	1479.0
38.00	1687.0
39.00	676.0
41.10	155.0
43.00	147.0
44.00	613.0
45.00	458.0
47.00	327.0
47.90	209.0
49.00	1466.0
50.00	7255.0
51.00	2227.0
51.90	143.0
54.80	174.0
55.90	794.0
57.00	1265.0
58.00	115.0
60.10	229.0
61.10	1755.0
62.00	2092.0
63.00	1595.0
63.90	113.0
66.80	185.0
68.00	4363.0
69.00	3997.0
70.00	421.0
71.80	202.0
73.00	1935.0
74.00	7058.0
75.00	19984.0
76.00	1924.0
76.90	289.0
77.80	105.0
78.90	1550.0
79.90	530.0
80.90	1805.0
81.90	503.0
86.90	1549.0
87.90	1543.0
90.90	227.0
91.90	1212.0
92.90	1814.0
94.00	4833.0
95.00	37544.0
96.00	2533.0
97.00	125.0
103.80	205.0
105.90	237.0
115.90	179.0
116.90	386.0
117.80	170.0
118.90	196.0
127.80	189.0
128.70	121.0
129.80	154.0
134.70	112.0
136.90	124.0
140.90	599.0
142.80	541.0
147.80	139.0
154.90	138.0
173.90	32208.0
174.90	2347.0
175.90	30672.0
176.90	1927.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

Scan 2796 (10.080 min): VV009314.D
BFB64

m/z	Abundance
38.90	114.0
39.90	168.0
41.00	169.0
42.90	169.0
43.90	406.0
53.10	105.0
54.90	134.0
57.00	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64