

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\
 Data File : VV014657.D
 Acq On : 21 Feb 2020 16:53
 Operator : SY/MD
 Sample : L1608-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.586	147	154	169	rVB	49480	58248	7.35%	1.040%
2	2.129	312	323	333	rBV	118207	166531	21.02%	2.972%
3	3.077	616	618	623	rVB2	591	330	0.04%	0.006%
4	3.103	623	626	630	rBV2	329	285	0.04%	0.005%
5	3.196	653	655	658	rBV2	268	151	0.02%	0.003%
6	3.280	680	681	684	rBV2	256	120	0.02%	0.002%
7	3.421	724	725	728	rVB2	205	69	0.01%	0.001%
8	3.444	730	732	734	rBV	287	126	0.02%	0.002%
9	3.576	772	773	775	rBV	324	124	0.02%	0.002%
10	3.589	775	777	778	rBV	229	72	0.01%	0.001%
11	3.746	821	826	833	rBV6	548	530	0.07%	0.009%
12	3.772	833	834	835	rBV6	312	93	0.01%	0.002%
13	3.849	856	858	860	rBV	196	76	0.01%	0.001%
14	3.865	860	863	864	rBV	342	151	0.02%	0.003%
15	3.897	872	873	877	rBV2	243	162	0.02%	0.003%
16	3.946	877	888	913	rBV2	43143	158850	20.05%	2.835%
17	4.650	1104	1107	1110	rBV2	560	330	0.04%	0.006%
18	4.688	1116	1119	1122	rBV2	302	175	0.02%	0.003%
19	4.798	1151	1153	1154	rBV2	383	135	0.02%	0.002%
20	4.846	1166	1168	1173	rBV2	362	270	0.03%	0.005%
21	4.923	1189	1192	1193	rBV	450	245	0.03%	0.004%
22	4.955	1199	1202	1204	rBV	351	168	0.02%	0.003%
23	5.090	1223	1244	1267	rBV2	314256	792368	100.00%	14.143%
24	5.489	1366	1368	1371	rVB	489	211	0.03%	0.004%
25	5.659	1409	1421	1444	rBV	258565	509881	64.35%	9.101%
26	6.113	1548	1562	1582	rBV	176421	357942	45.17%	6.389%
27	6.572	1704	1705	1706	rBV	115	25	0.00%	0.000%
28	6.579	1706	1707	1711	rVB	215	100	0.01%	0.002%
29	6.608	1711	1716	1719	rBV3	689	585	0.07%	0.010%
30	6.720	1749	1751	1753	rBV	298	168	0.02%	0.003%
31	6.791	1770	1773	1774	rBV2	516	238	0.03%	0.004%
32	6.878	1796	1800	1802	rBV	283	222	0.03%	0.004%
33	6.917	1809	1812	1813	rBV	220	116	0.01%	0.002%
34	6.965	1823	1827	1829	rBV2	403	264	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\
 Data File : VV014657.D
 Acq On : 21 Feb 2020 16:53
 Operator : SY/MD
 Sample : L1608-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis

35	7.026	1836	1846	1863	rBV	104052	182875	23.08%	3.264%
36	7.280	1924	1925	1927	rBV	376	140	0.02%	0.002%
37	7.302	1931	1932	1933	rBV	195	61	0.01%	0.001%
38	7.354	1936	1948	1969	rBV	379716	661456	83.48%	11.807%
39	7.659	2032	2043	2062	rBV	75531	130337	16.45%	2.326%
40	7.830	2093	2096	2098	rVB	310	173	0.02%	0.003%
41	7.852	2098	2103	2105	rBV2	436	410	0.05%	0.007%
42	7.871	2107	2109	2111	rVV	455	154	0.02%	0.003%
43	8.035	2158	2160	2161	rBV	255	70	0.01%	0.001%
44	8.064	2166	2169	2172	rBV3	261	194	0.02%	0.003%
45	8.077	2172	2173	2175	rBV3	350	151	0.02%	0.003%
46	8.135	2180	2191	2223	rBV	172764	359074	45.32%	6.409%
47	8.537	2315	2316	2317	rBV	327	89	0.01%	0.002%
48	8.630	2342	2345	2348	rBV	502	263	0.03%	0.005%
49	8.801	2396	2398	2399	rBV	350	189	0.02%	0.003%
50	8.891	2414	2426	2447	rBV	375772	614476	77.55%	10.968%
51	9.138	2499	2503	2505	rBV2	558	388	0.05%	0.007%
52	9.257	2538	2540	2541	rBV	458	232	0.03%	0.004%
53	9.293	2550	2551	2554	rBV	205	102	0.01%	0.002%
54	9.331	2561	2563	2566	rBV	430	234	0.03%	0.004%
55	9.347	2566	2568	2571	rVB	671	269	0.03%	0.005%
56	9.399	2581	2584	2585	rBV	260	106	0.01%	0.002%
57	9.434	2593	2595	2598	rBV	380	248	0.03%	0.004%
58	9.540	2625	2628	2631	rBV2	334	199	0.03%	0.004%
59	9.624	2652	2654	2656	rBV	367	142	0.02%	0.003%
60	9.695	2672	2676	2678	rBV2	495	232	0.03%	0.004%
61	9.730	2684	2687	2689	rBV3	522	286	0.04%	0.005%
62	9.852	2723	2725	2727	rVB	327	141	0.02%	0.003%
63	10.000	2769	2771	2773	rBV2	221	139	0.02%	0.002%
64	10.138	2810	2814	2817	rBV3	386	300	0.04%	0.005%
65	10.203	2833	2834	2835	rBV3	245	87	0.01%	0.002%
66	10.254	2838	2850	2863	rBV	246818	387254	48.87%	6.912%
67	10.322	2870	2871	2875	rBV2	642	343	0.04%	0.006%
68	10.415	2898	2900	2901	rBV2	318	157	0.02%	0.003%
69	10.447	2909	2910	2912	rBV	297	117	0.01%	0.002%
70	10.469	2915	2917	2920	rBV2	589	278	0.04%	0.005%
71	10.704	2988	2990	2992	rVB2	313	93	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\
 Data File : VV014657.D
 Acq On : 21 Feb 2020 16:53
 Operator : SY/MD
 Sample : L1608-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis

72	10.772	3010	3011	3012	rBV	244	81	0.01%	0.001%
73	11.013	3084	3086	3088	rBV	315	134	0.02%	0.002%
74	11.090	3108	3110	3112	rBV	496	285	0.04%	0.005%
75	11.148	3126	3128	3133	rVB	463	279	0.04%	0.005%
76	11.215	3145	3149	3151	rBV3	715	523	0.07%	0.009%
77	11.286	3161	3171	3186	rBV	379037	594843	75.07%	10.618%
78	11.666	3276	3289	3309	rBV	385223	611599	77.19%	10.917%
79	12.055	3409	3410	3411	rBV	123	38	0.00%	0.001%
80	12.183	3449	3450	3454	rBV	291	163	0.02%	0.003%
81	12.370	3505	3508	3509	rVB	271	108	0.01%	0.002%
82	12.540	3560	3561	3562	rBV	220	46	0.01%	0.001%
83	12.547	3562	3563	3567	rVV	463	169	0.02%	0.003%
84	12.714	3614	3615	3616	rBV	290	59	0.01%	0.001%
85	12.804	3642	3643	3645	rBV2	408	147	0.02%	0.003%
86	12.842	3653	3655	3657	rBV	307	130	0.02%	0.002%
87	12.855	3657	3659	3661	rVV	510	217	0.03%	0.004%
88	12.871	3662	3664	3666	rVV	391	125	0.02%	0.002%
89	12.919	3677	3679	3681	rVB2	460	161	0.02%	0.003%
90	13.444	3840	3842	3843	rBV2	263	80	0.01%	0.001%
91	13.598	3889	3890	3895	rBV2	562	315	0.04%	0.006%
92	13.788	3946	3949	3953	rBV2	610	571	0.07%	0.010%
93	13.874	3973	3976	3979	rBV3	415	280	0.04%	0.005%
94	14.177	4068	4070	4074	rBV2	415	281	0.04%	0.005%
95	14.411	4141	4143	4145	rBV	423	281	0.04%	0.005%
96	14.505	4167	4172	4176	rBV3	410	396	0.05%	0.007%
97	14.852	4278	4280	4284	rBV2	493	308	0.04%	0.005%


Sum of corrected areas: 5602439

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022120\
Data File : VV014657.D
Acq On : 21 Feb 2020 16:53
Operator : SY/MD
Sample : L1608-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

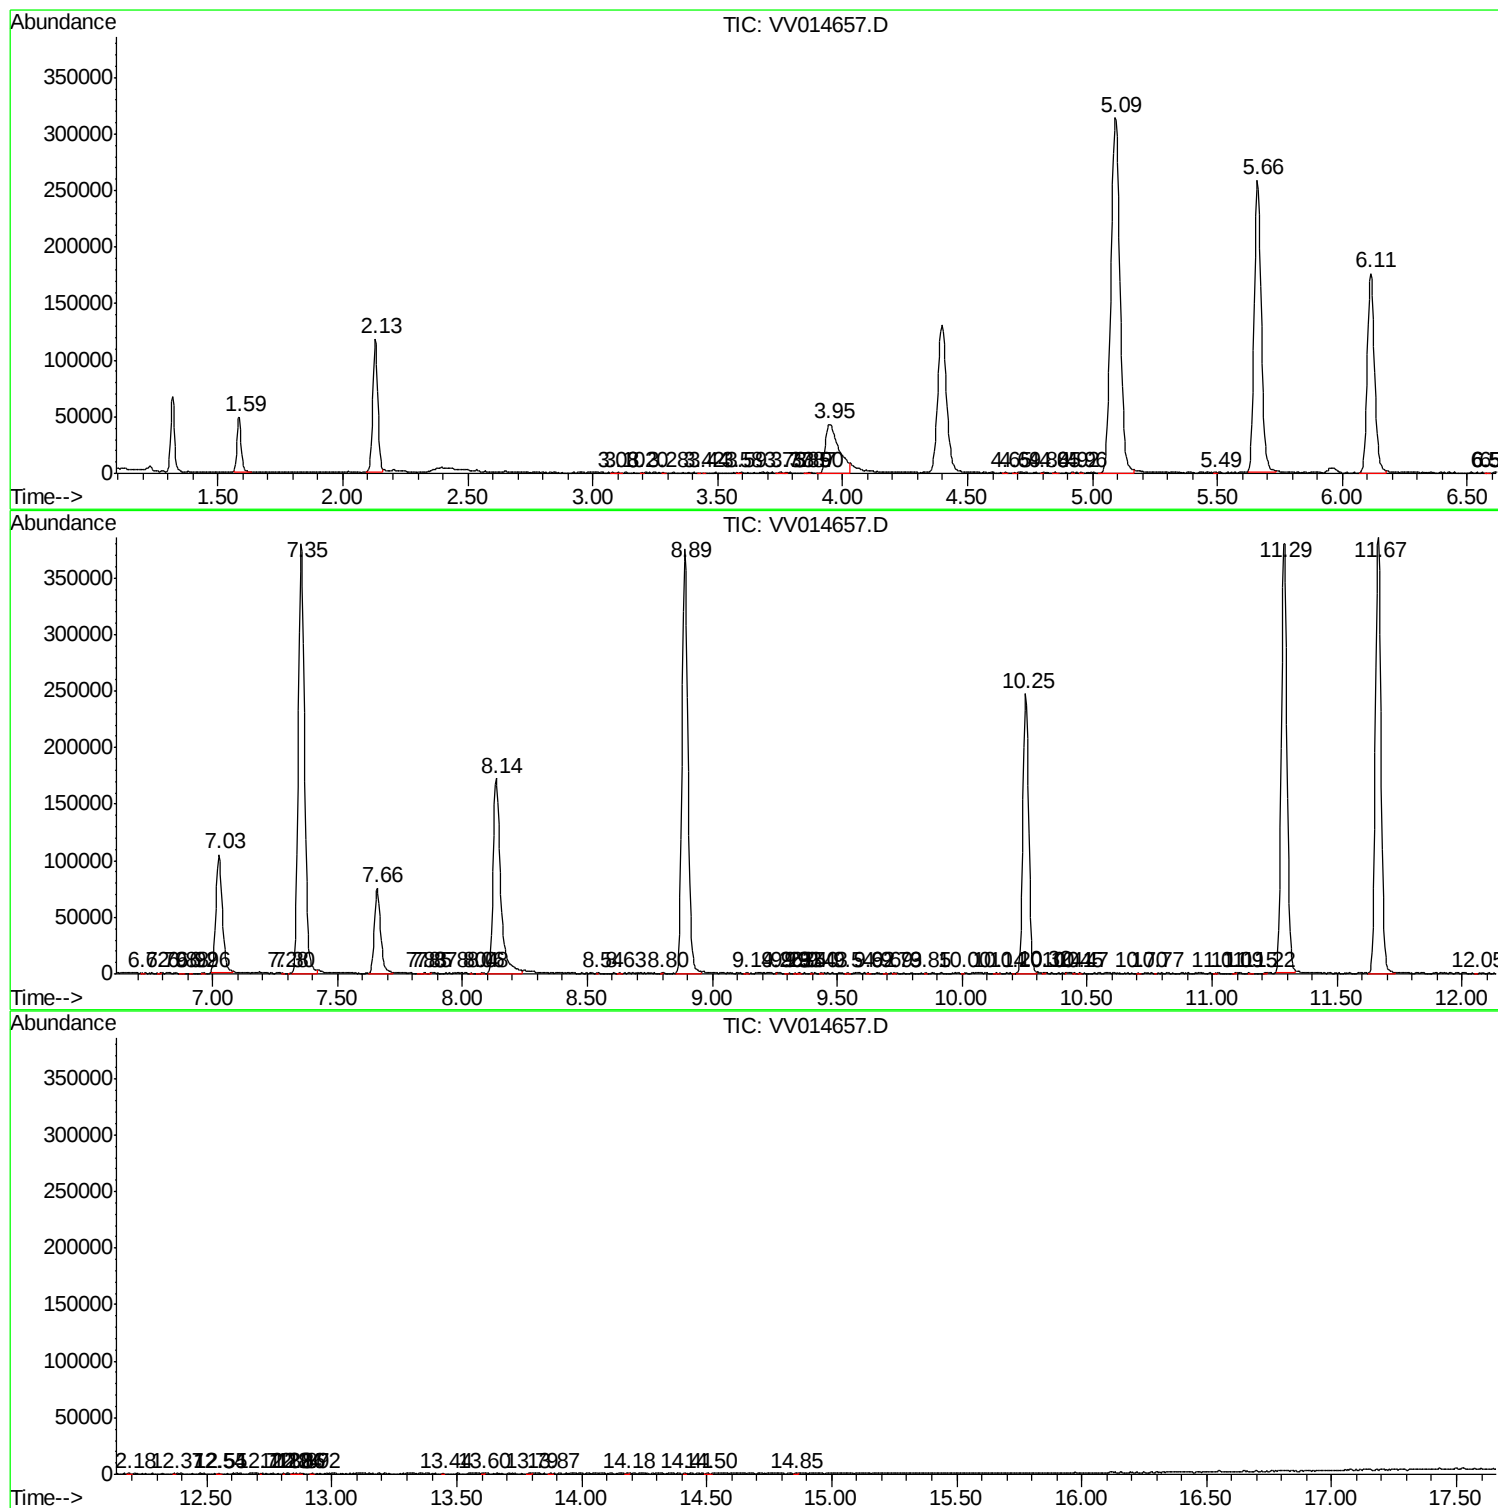

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022120\
Data File : VV014657.D
Acq On : 21 Feb 2020 16:53
Operator : SY/MD
Sample : L1608-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022120\
Data File : VV014657.D
Acq On : 21 Feb 2020 16:53
Operator : SY/MD
Sample : L1608-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
