

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\
 Data File : VV014658.D
 Acq On : 21 Feb 2020 17:16
 Operator : SY/MD
 Sample : L1608-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.585	146	154	174	rBV	49735	62354	7.69%	1.083%
2	2.132	313	324	335	rBV	120199	172039	21.21%	2.988%
3	2.878	554	556	558	rBV2	285	160	0.02%	0.003%
4	2.929	570	572	574	rBV	307	191	0.02%	0.003%
5	3.132	633	635	637	rVB2	430	194	0.02%	0.003%
6	3.148	638	640	641	rBV	395	127	0.02%	0.002%
7	3.235	664	667	668	rBV	283	127	0.02%	0.002%
8	3.560	765	768	769	rBV	356	191	0.02%	0.003%
9	3.675	801	804	810	rVB2	620	552	0.07%	0.010%
10	3.907	872	876	878	rBV	408	322	0.04%	0.006%
11	3.952	878	890	926	rBV	42417	171480	21.14%	2.978%
12	4.617	1096	1097	1098	rBV	294	97	0.01%	0.002%
13	5.093	1227	1245	1272	rBV2	323556	810981	100.00%	14.085%
14	5.354	1324	1326	1329	rVB	363	139	0.02%	0.002%
15	5.437	1349	1352	1353	rBV2	603	266	0.03%	0.005%
16	5.592	1397	1400	1403	rBV3	406	335	0.04%	0.006%
17	5.659	1408	1421	1444	rBV	269955	532978	65.72%	9.256%
18	6.113	1548	1562	1592	rBV	179942	366241	45.16%	6.361%
19	6.418	1654	1657	1660	rBV2	469	373	0.05%	0.006%
20	6.463	1669	1671	1675	rVB3	687	362	0.04%	0.006%
21	6.482	1675	1677	1680	rBV2	170	82	0.01%	0.001%
22	6.498	1680	1682	1683	rBV	365	119	0.01%	0.002%
23	6.627	1718	1722	1723	rBV2	841	519	0.06%	0.009%
24	6.846	1787	1790	1793	rBV2	278	188	0.02%	0.003%
25	7.026	1835	1846	1868	rBV2	108965	196542	24.24%	3.413%
26	7.293	1927	1929	1931	rBV2	435	215	0.03%	0.004%
27	7.357	1935	1949	1977	rBV	387627	681668	84.05%	11.839%
28	7.659	2034	2043	2060	rBV	76237	127942	15.78%	2.222%
29	7.833	2093	2097	2099	rBV2	443	311	0.04%	0.005%
30	7.913	2120	2122	2124	rBV2	390	229	0.03%	0.004%
31	7.942	2128	2131	2133	rBV3	342	175	0.02%	0.003%
32	8.042	2159	2162	2168	rVB3	794	588	0.07%	0.010%
33	8.077	2169	2173	2177	rBV3	556	477	0.06%	0.008%
34	8.135	2180	2191	2217	rBV	174508	355835	43.88%	6.180%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\
 Data File : VV014658.D
 Acq On : 21 Feb 2020 17:16
 Operator : SY/MD
 Sample : L1608-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis

35	8.662	2353	2355	2357	rBV2	523	270	0.03%	0.005%
36	8.678	2357	2360	2362	rBV2	216	139	0.02%	0.002%
37	8.788	2393	2394	2398	rVB2	509	134	0.02%	0.002%
38	8.817	2401	2403	2407	rBV2	586	382	0.05%	0.007%
39	8.833	2407	2408	2410	rBV	204	78	0.01%	0.001%
40	8.891	2414	2426	2447	rBV	391319	633806	78.15%	11.008%
41	9.129	2498	2500	2502	rBV	392	195	0.02%	0.003%
42	9.312	2555	2557	2561	rVB2	612	286	0.04%	0.005%
43	9.347	2566	2568	2570	rBV	563	238	0.03%	0.004%
44	9.434	2593	2595	2597	rBV	510	212	0.03%	0.004%
45	9.563	2633	2635	2637	rBV	332	158	0.02%	0.003%
46	9.701	2676	2678	2682	rVB	202	77	0.01%	0.001%
47	9.730	2685	2687	2689	rBV2	398	215	0.03%	0.004%
48	9.823	2714	2716	2718	rVB2	740	226	0.03%	0.004%
49	9.836	2718	2720	2723	rBV	323	139	0.02%	0.002%
50	10.254	2839	2850	2865	rBV	249210	391714	48.30%	6.803%
51	10.460	2912	2914	2915	rBV	241	99	0.01%	0.002%
52	10.563	2944	2946	2949	rBV	457	203	0.03%	0.004%
53	10.791	3016	3017	3022	rVB2	337	161	0.02%	0.003%
54	10.852	3034	3036	3043	rBV2	314	241	0.03%	0.004%
55	11.289	3161	3172	3190	rBV	400454	620062	76.46%	10.769%
56	11.665	3277	3289	3307	rBV	395280	623656	76.90%	10.831%
57	12.058	3409	3411	3413	rBV2	274	134	0.02%	0.002%
58	12.132	3432	3434	3437	rVB2	325	134	0.02%	0.002%
59	12.312	3488	3490	3493	rBV2	523	304	0.04%	0.005%
60	12.839	3652	3654	3656	rBV2	362	121	0.01%	0.002%
61	14.559	4187	4189	4190	rBV	383	159	0.02%	0.003%


Sum of corrected areas: 5757942

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022120\
Data File : VV014658.D
Acq On : 21 Feb 2020 17:16
Operator : SY/MD
Sample : L1608-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

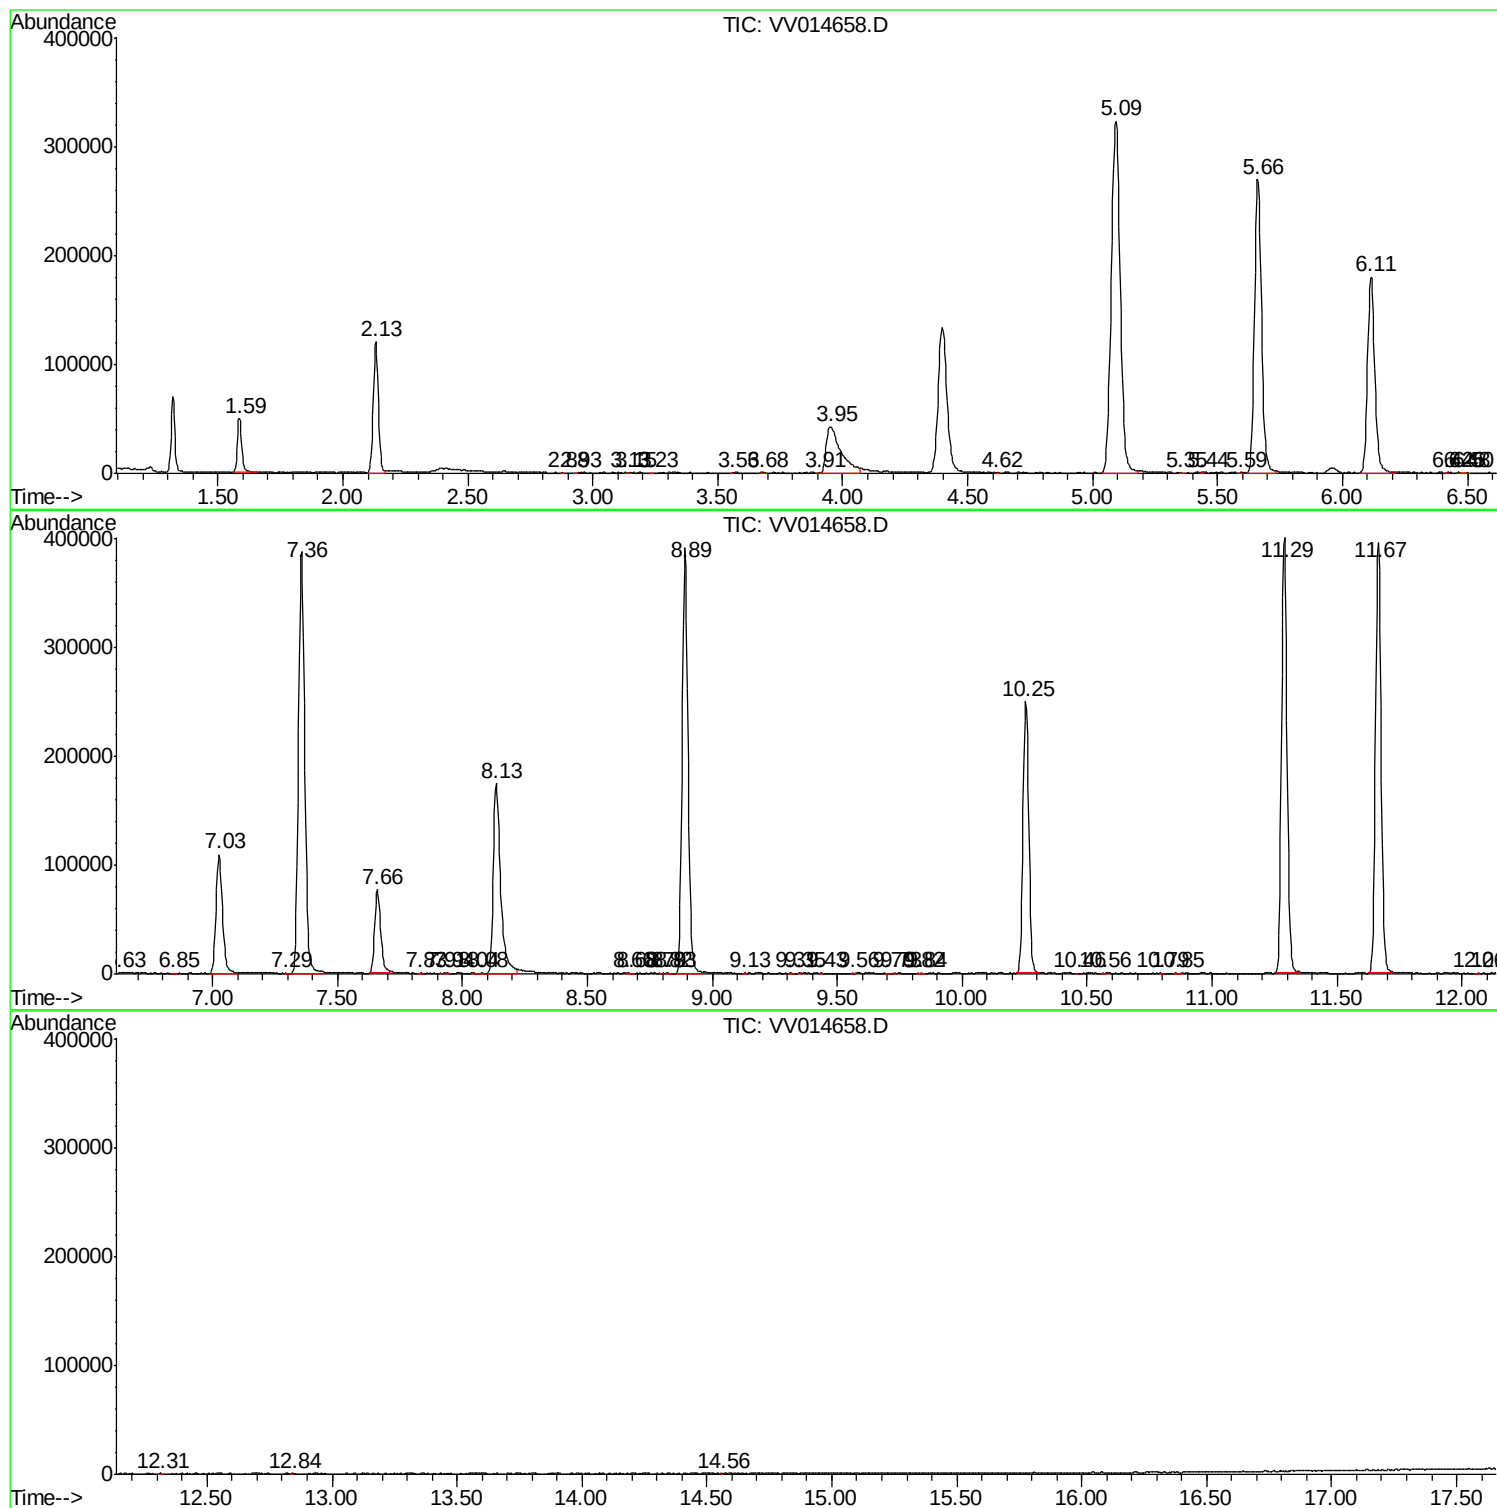

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022120\
Data File : VV014658.D
Acq On : 21 Feb 2020 17:16
Operator : SY/MD
Sample : L1608-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022120\
Data File : VV014658.D
Acq On : 21 Feb 2020 17:16
Operator : SY/MD
Sample : L1608-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc