

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\  
 Data File : VV014665.D  
 Acq On : 21 Feb 2020 19:59  
 Operator : SY/MD  
 Sample : L1607-13  
 Misc : 5.0mL/MSVOA V/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampled :  
 C0AP9

Integration Parameters: LSCINT.P

Integrator: RTE  
 Smoothing : OFF  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0

Filtering: 5  
 Min Area: 0 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM022120WMA.M  
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	66	71	85	rVB	63898	62907	3.82%	0.891%
2	1.585	148	154	169	rVB	49010	56312	3.42%	0.797%
3	1.978	272	276	279	rBV3	901	786	0.05%	0.011%
4	2.036	290	294	295	rBV2	437	303	0.02%	0.004%
5	2.081	305	308	309	rBV2	396	186	0.01%	0.003%
6	2.129	315	323	339	rVB	113972	165993	10.07%	2.351%
7	3.100	621	625	626	rBV	639	399	0.02%	0.006%
8	3.196	654	655	656	rBV	227	76	0.00%	0.001%
9	3.338	697	699	702	rVB2	418	186	0.01%	0.003%
10	3.389	714	715	716	rBV	114	25	0.00%	0.000%
11	3.399	716	718	719	rBV	320	104	0.01%	0.001%
12	3.431	725	728	732	rBV	316	257	0.02%	0.004%
13	3.502	747	750	751	rBV	362	184	0.01%	0.003%
14	3.704	809	813	816	rBV	330	285	0.02%	0.004%
15	3.804	842	844	846	rBV	231	76	0.00%	0.001%
16	3.855	858	860	862	rBV	439	185	0.01%	0.003%
17	3.958	878	892	922	rBV3	120860	345368	20.95%	4.891%
18	4.820	1159	1160	1162	rBV	339	126	0.01%	0.002%
19	4.884	1179	1180	1182	rBV	242	98	0.01%	0.001%
20	4.990	1211	1213	1214	rBV	224	79	0.00%	0.001%
21	5.093	1226	1245	1275	rBV2	303826	771041	46.76%	10.919%
22	5.360	1326	1328	1329	rBV	349	134	0.01%	0.002%
23	5.405	1341	1342	1343	rBV	425	92	0.01%	0.001%
24	5.659	1408	1421	1444	rBV	260097	514751	31.22%	7.289%
25	5.955	1498	1513	1543	rBV	860241	1648898	100.00%	23.350%
26	6.444	1664	1665	1666	rVB	278	54	0.00%	0.001%
27	6.479	1675	1676	1677	rBV	367	106	0.01%	0.002%
28	6.769	1764	1766	1769	rVB	174	54	0.00%	0.001%
29	6.794	1769	1774	1775	rBV	276	205	0.01%	0.003%
30	6.878	1798	1800	1801	rBV	314	144	0.01%	0.002%
31	6.958	1824	1825	1826	rBV	376	125	0.01%	0.002%
32	7.026	1834	1846	1864	rBV	102764	184332	11.18%	2.610%
33	7.190	1894	1897	1898	rBV2	750	452	0.03%	0.006%
34	7.305	1930	1933	1936	rBV	449	219	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\  
 Data File : VV014665.D  
 Acq On : 21 Feb 2020 19:59  
 Operator : SY/MD  
 Sample : L1607-13  
 Misc : 5.0mL/MSVOA V/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AP9

## Integration Parameters: LSCINT.P

Integrator: RTE  
 Smoothing : OFF  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0

Filtering: 5  
 Min Area: 0 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM022120WMA.M  
 Title : VOC Analysis

35	7.357	1936	1949	1967	rBV	368175	641938	38.93%	9.090%
36	7.659	2033	2043	2062	rBV	72660	122276	7.42%	1.732%
37	8.135	2181	2191	2219	rBV3	158609	336144	20.39%	4.760%
38	8.534	2311	2315	2317	rBV2	429	298	0.02%	0.004%
39	8.640	2346	2348	2350	rBV2	510	205	0.01%	0.003%
40	8.694	2363	2365	2368	rBV	282	164	0.01%	0.002%
41	8.717	2370	2372	2373	rBV	303	104	0.01%	0.001%
42	8.804	2397	2399	2400	rVB	572	146	0.01%	0.002%
43	8.833	2405	2408	2411	rBV3	386	301	0.02%	0.004%
44	8.891	2415	2426	2448	rVV	379256	617180	37.43%	8.740%
45	9.106	2491	2493	2494	rBV	253	103	0.01%	0.001%
46	9.174	2512	2514	2515	rBV	655	245	0.01%	0.003%
47	9.225	2529	2530	2532	rBV2	348	161	0.01%	0.002%
48	9.305	2553	2555	2557	rVB2	637	222	0.01%	0.003%
49	9.328	2559	2562	2564	rVB2	361	214	0.01%	0.003%
50	9.476	2607	2608	2611	rVB	192	63	0.00%	0.001%
51	9.502	2613	2616	2620	rVV2	454	249	0.02%	0.004%
52	9.547	2629	2630	2633	rBV2	294	119	0.01%	0.002%
53	9.749	2690	2693	2695	rBV	451	264	0.02%	0.004%
54	10.090	2797	2799	2803	rVB	524	357	0.02%	0.005%
55	10.154	2817	2819	2823	rVB	252	164	0.01%	0.002%
56	10.174	2823	2825	2826	rBV	198	66	0.00%	0.001%
57	10.254	2839	2850	2865	rBV	242204	376424	22.83%	5.331%
58	10.350	2878	2880	2887	rVB2	468	325	0.02%	0.005%
59	10.379	2887	2889	2893	rBV	454	247	0.01%	0.003%
60	10.604	2957	2959	2961	rVB2	297	98	0.01%	0.001%
61	10.630	2966	2967	2971	rVB2	285	108	0.01%	0.002%
62	10.653	2971	2974	2975	rBV	256	128	0.01%	0.002%
63	10.755	3005	3006	3008	rBV2	349	141	0.01%	0.002%
64	10.807	3020	3022	3025	rBV	622	290	0.02%	0.004%
65	11.029	3087	3091	3093	rBV	552	307	0.02%	0.004%
66	11.177	3134	3137	3138	rBV2	392	193	0.01%	0.003%
67	11.212	3147	3148	3149	rBV2	325	110	0.01%	0.002%
68	11.289	3161	3172	3193	rBV	391724	605927	36.75%	8.581%
69	11.665	3277	3289	3309	rBV	376181	598556	36.30%	8.476%
70	11.878	3354	3355	3357	rBV	260	129	0.01%	0.002%
71	11.935	3371	3373	3375	rBV2	320	167	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\  
Data File : VV014665.D  
Acq On : 21 Feb 2020 19:59  
Operator : SY/MD  
Sample : L1607-13  
Misc : 5.0mL/MSVOA V/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AP9

Integration Parameters: LSCINT.P  
Integrator: RTE  
Smoothing : OFF Filtering: 5  
Sampling : 1 Min Area: 0 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM022120WMA.M  
Title : VOC Analysis

72	12.640	3589	3592	3595	rBV2	252	188	0.01%	0.003%
73	12.662	3595	3599	3601	rBV2	476	366	0.02%	0.005%
74	12.910	3673	3676	3678	rBV2	377	239	0.01%	0.003%
75	13.006	3700	3706	3708	rBV2	427	382	0.02%	0.005%
76	13.029	3711	3713	3714	rBV	309	97	0.01%	0.001%
77	13.411	3829	3832	3836	rBV	632	457	0.03%	0.006%
78	13.919	3986	3990	3994	rBV2	481	362	0.02%	0.005%
79	14.119	4050	4052	4055	rBV2	460	311	0.02%	0.004%
80	14.903	4292	4296	4300	rBV3	596	569	0.03%	0.008%




Sum of corrected areas: 7061646

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\  
 Data File : VV014665.D  
 Acq On : 21 Feb 2020 19:59  
 Operator : SY/MD  
 Sample : L1607-13  
 Misc : 5.0mL/MSVOA V/WATER  
 ALS Vial : 24 Sample Multiplier: 1

**Instrument :**  
 MSVOA\_V  
**ClientSampleId :**  
 C0AP9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM022120WMA.M  
 Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L  
 TIC Integration Parameters: LSCINT.P

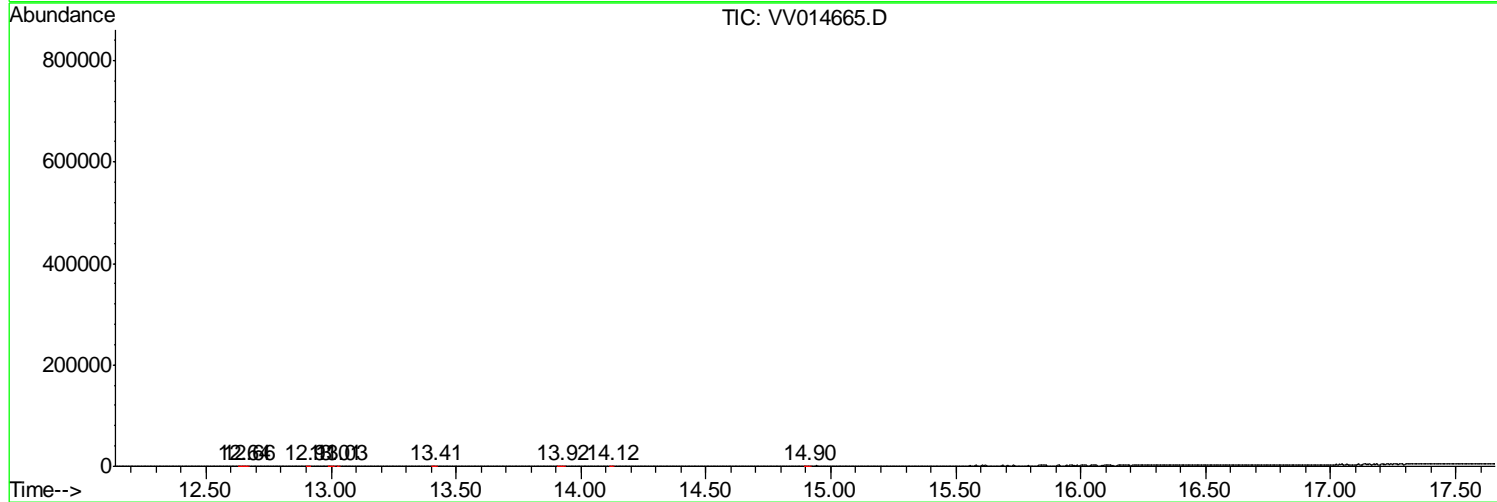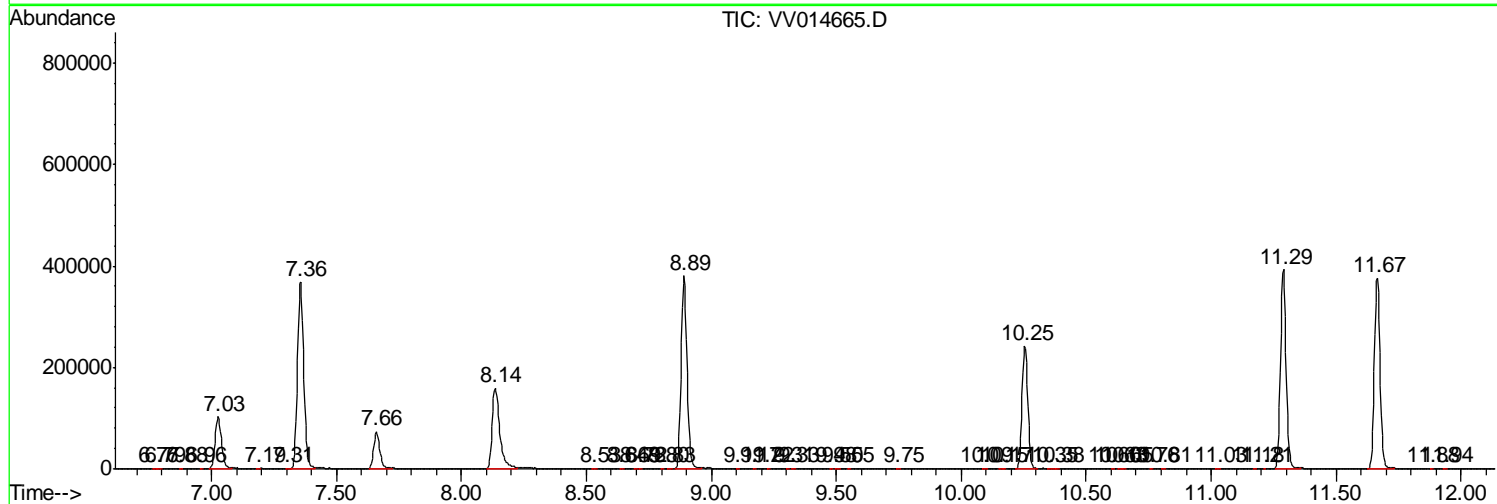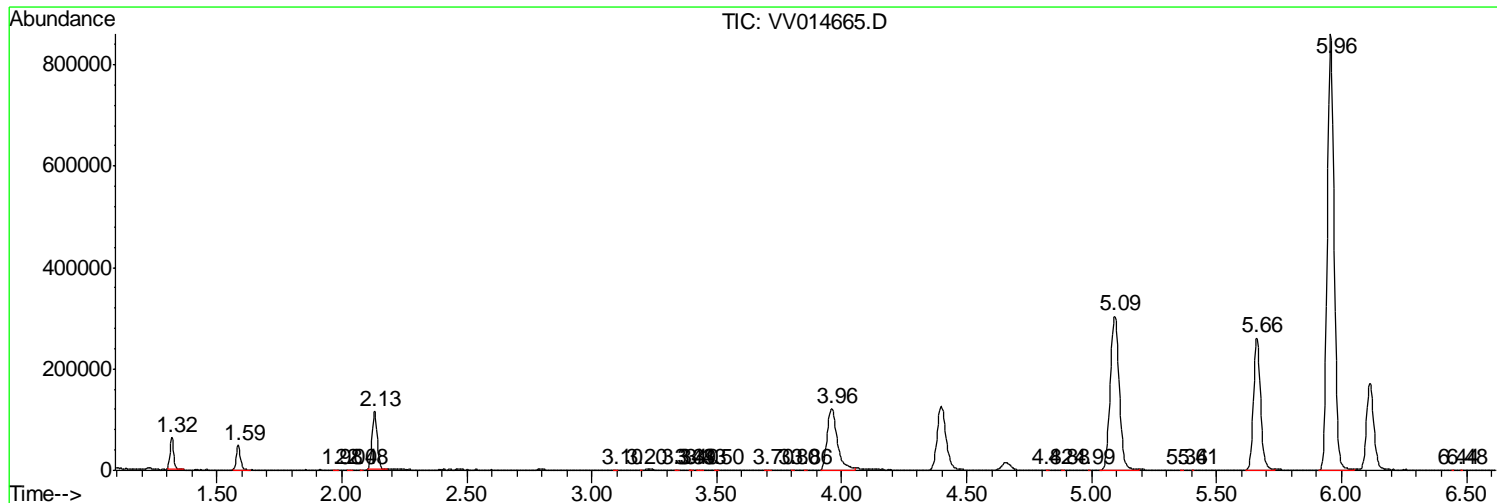

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_V\DATA\VV022120\  
Data File : VV014665.D  
Acq On : 21 Feb 2020 19:59  
Operator : SY/MD  
Sample : L1607-13  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AP9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM022120WMA.M  
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_V\DATA\VV022120\  
Data File : VV014665.D  
Acq On : 21 Feb 2020 19:59  
Operator : SY/MD  
Sample : L1607-13  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AP9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM022120WMA.M  
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc

---