

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\
 Data File : VV014674.D
 Acq On : 21 Feb 2020 23:52
 Operator : SY/MD
 Sample : L1608-01 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	86	rVB	58351	61319	8.04%	1.136%
2	1.586	147	154	169	rVB	45220	53898	7.07%	0.998%
3	2.315	377	381	384	rBV3	921	634	0.08%	0.012%
4	2.772	522	523	525	rBV	301	140	0.02%	0.003%
5	3.817	843	848	852	rBV3	437	444	0.06%	0.008%
6	3.891	870	871	873	rBV	389	161	0.02%	0.003%
7	3.955	879	891	914	rBV2	38371	137638	18.04%	2.550%
8	4.897	1183	1184	1186	rBV	221	102	0.01%	0.002%
9	5.013	1218	1220	1221	rVB2	280	68	0.01%	0.001%
10	5.029	1221	1225	1227	rBV	544	344	0.05%	0.006%
11	5.093	1227	1245	1269	rBV2	303620	762825	100.00%	14.131%
12	5.614	1405	1407	1408	rBV	342	113	0.01%	0.002%
13	5.659	1410	1421	1450	rVB	258912	512419	67.17%	9.492%
14	5.907	1495	1498	1502	rBV2	538	441	0.06%	0.008%
15	5.962	1503	1515	1533	rVB5	21705	45580	5.98%	0.844%
16	6.113	1549	1562	1581	rBV	169524	341903	44.82%	6.334%
17	6.534	1691	1693	1698	rBV2	246	235	0.03%	0.004%
18	6.553	1698	1699	1704	rVV2	385	248	0.03%	0.005%
19	6.907	1807	1809	1812	rBV	444	239	0.03%	0.004%
20	6.942	1817	1820	1824	rBV2	532	382	0.05%	0.007%
21	6.962	1824	1826	1829	rBV2	371	241	0.03%	0.004%
22	7.026	1835	1846	1868	rBV2	98861	178010	23.34%	3.298%
23	7.286	1926	1927	1929	rBV	536	200	0.03%	0.004%
24	7.357	1937	1949	1974	rBV	366525	637108	83.52%	11.802%
25	7.659	2033	2043	2065	rBV	71978	122929	16.11%	2.277%
26	8.055	2164	2166	2169	rBV2	370	196	0.03%	0.004%
27	8.068	2169	2170	2171	rBV	248	81	0.01%	0.002%
28	8.135	2180	2191	2213	rBV2	162670	333780	43.76%	6.183%
29	8.704	2362	2368	2372	rBV2	448	551	0.07%	0.010%
30	8.891	2414	2426	2446	rBV	384792	616243	80.78%	11.415%
31	9.142	2502	2504	2507	rVB2	404	139	0.02%	0.003%
32	9.341	2564	2566	2570	rBV2	467	253	0.03%	0.005%
33	9.540	2626	2628	2631	rBV	313	123	0.02%	0.002%
34	9.633	2655	2657	2660	rBV2	485	231	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\
 Data File : VV014674.D
 Acq On : 21 Feb 2020 23:52
 Operator : SY/MD
 Sample : L1608-01 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis

35	9.749	2692	2693	2694	rBV2	234	74	0.01%	0.001%
36	9.775	2698	2701	2703	rBV2	266	154	0.02%	0.003%
37	9.810	2710	2712	2713	rBV	247	65	0.01%	0.001%
38	9.862	2725	2728	2731	rBV2	244	181	0.02%	0.003%
39	10.254	2839	2850	2865	rBV	240607	375363	49.21%	6.953%
40	10.733	2996	2999	3003	rBV2	401	299	0.04%	0.006%
41	11.080	3106	3107	3109	rVB	263	70	0.01%	0.001%
42	11.190	3140	3141	3143	rBV	406	145	0.02%	0.003%
43	11.289	3160	3172	3193	rBV	386897	607309	79.61%	11.250%
44	11.666	3277	3289	3306	rBV	380638	603661	79.13%	11.182%
45	12.318	3490	3492	3497	rBV2	400	292	0.04%	0.005%
46	12.431	3525	3527	3531	rVB2	426	289	0.04%	0.005%
47	12.720	3615	3617	3618	rBV	325	100	0.01%	0.002%
48	13.225	3772	3774	3777	rBV	271	141	0.02%	0.003%
49	13.260	3780	3785	3786	rBV2	304	233	0.03%	0.004%
50	13.948	3995	3999	4004	rVB3	599	508	0.07%	0.009%
51	14.074	4037	4038	4042	rVB	537	211	0.03%	0.004%


Sum of corrected areas: 5398313

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022120\
Data File : VV014674.D
Acq On : 21 Feb 2020 23:52
Operator : SY/MD
Sample : L1608-01 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

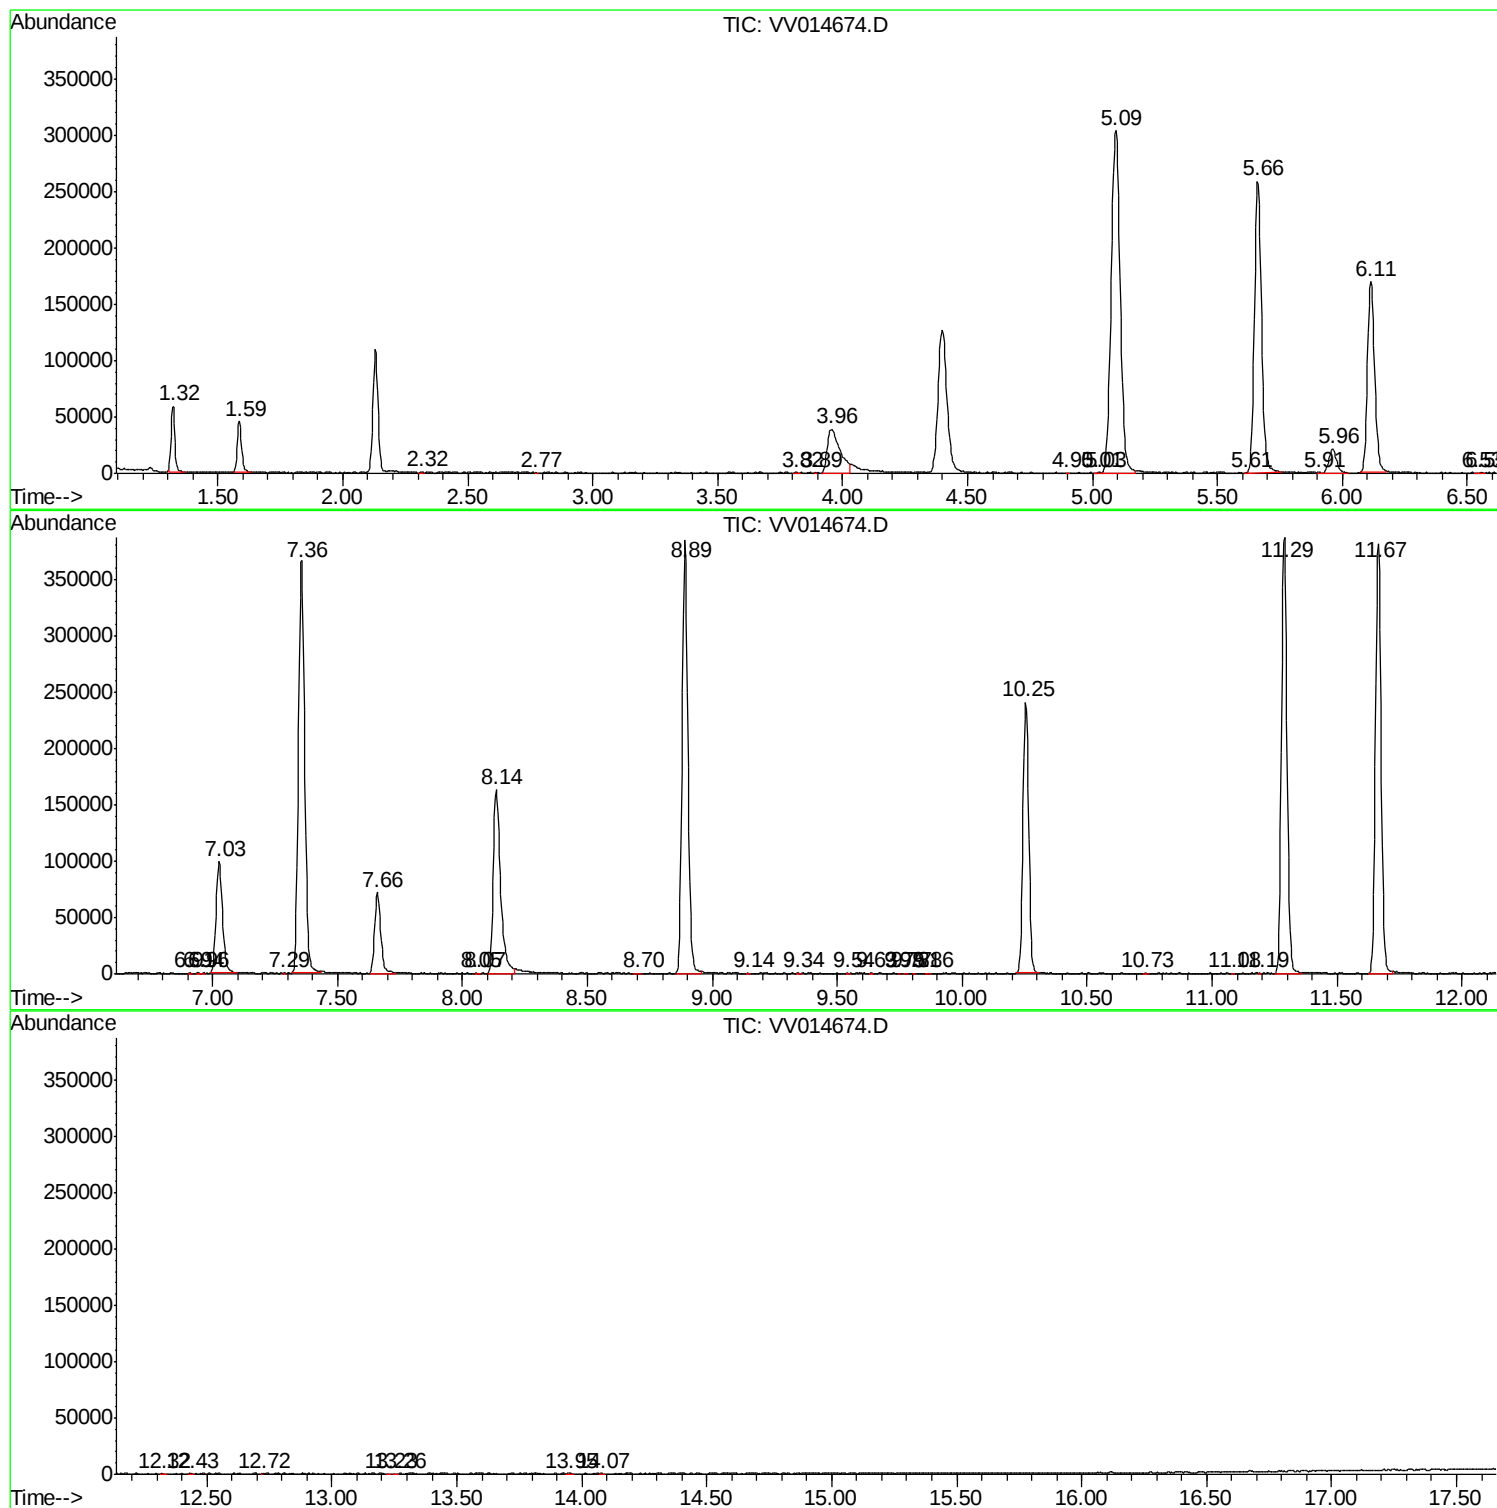

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022120\
Data File : VV014674.D
Acq On : 21 Feb 2020 23:52
Operator : SY/MD
Sample : L1608-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022120\
Data File : VV014674.D
Acq On : 21 Feb 2020 23:52
Operator : SY/MD
Sample : L1608-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc