

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\
 Data File : VV014677.D
 Acq On : 22 Feb 2020 01:02
 Operator : SY/MD
 Sample : L1608-08 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	82	rVB	55394	56986	7.81%	1.084%
2	1.585	147	154	168	rBV	43410	51734	7.09%	0.984%
3	2.039	291	295	298	rBV3	635	479	0.07%	0.009%
4	2.074	304	306	309	rBV2	468	370	0.05%	0.007%
5	2.129	313	323	334	rBV	102398	147516	20.22%	2.805%
6	2.791	527	529	533	rBV3	449	202	0.03%	0.004%
7	2.878	555	556	558	rVB	464	133	0.02%	0.003%
8	2.974	583	586	587	rBV	566	299	0.04%	0.006%
9	3.109	624	628	629	rBV	387	233	0.03%	0.004%
10	3.161	642	644	645	rBV	337	153	0.02%	0.003%
11	3.254	670	673	676	rBV2	425	302	0.04%	0.006%
12	3.547	762	764	769	rBV2	257	120	0.02%	0.002%
13	3.733	820	822	826	rBV2	305	214	0.03%	0.004%
14	3.752	826	828	829	rVB	372	94	0.01%	0.002%
15	3.765	829	832	834	rBV	428	245	0.03%	0.005%
16	3.862	860	862	863	rBV	222	98	0.01%	0.002%
17	3.958	878	892	934	rBV2	36485	152855	20.96%	2.906%
18	4.579	1083	1085	1087	rBV2	459	230	0.03%	0.004%
19	4.942	1196	1198	1199	rBV	304	134	0.02%	0.003%
20	5.093	1228	1245	1268	rBV2	289928	729402	100.00%	13.869%
21	5.331	1317	1319	1320	rBV2	383	140	0.02%	0.003%
22	5.518	1374	1377	1379	rVB3	399	197	0.03%	0.004%
23	5.592	1398	1400	1403	rBV2	463	276	0.04%	0.005%
24	5.659	1408	1421	1443	rBV	251792	496197	68.03%	9.435%
25	5.904	1495	1497	1498	rBV	399	192	0.03%	0.004%
26	6.113	1548	1562	1584	rBV	164168	334408	45.85%	6.358%
27	6.608	1714	1716	1718	rBV	316	154	0.02%	0.003%
28	7.026	1834	1846	1868	rBV	96288	173172	23.74%	3.293%
29	7.183	1894	1895	1897	rBV	458	181	0.02%	0.003%
30	7.209	1897	1903	1904	rBV3	605	428	0.06%	0.008%
31	7.357	1936	1949	1970	rBV	339953	597184	81.87%	11.355%
32	7.659	2033	2043	2066	rBV	68967	117624	16.13%	2.236%
33	8.022	2153	2156	2157	rBV	321	160	0.02%	0.003%
34	8.135	2181	2191	2221	rBV2	153655	322404	44.20%	6.130%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\
 Data File : VV014677.D
 Acq On : 22 Feb 2020 01:02
 Operator : SY/MD
 Sample : L1608-08 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis

35	8.569	2319	2326	2328	rBV3	565	648	0.09%	0.012%
36	8.682	2358	2361	2365	rBV3	748	604	0.08%	0.011%
37	8.788	2392	2394	2395	rBV	520	165	0.02%	0.003%
38	8.891	2414	2426	2444	rBV	364367	587663	80.57%	11.174%
39	9.219	2526	2528	2530	rBV	362	168	0.02%	0.003%
40	9.289	2548	2550	2551	rBV	252	63	0.01%	0.001%
41	9.341	2565	2566	2567	rBV	310	78	0.01%	0.001%
42	9.360	2570	2572	2574	rVB	156	41	0.01%	0.001%
43	9.373	2574	2576	2579	rBV	386	188	0.03%	0.004%
44	9.608	2647	2649	2651	rBV	470	237	0.03%	0.005%
45	9.656	2662	2664	2665	rBV	282	149	0.02%	0.003%
46	9.707	2676	2680	2681	rBV2	289	183	0.03%	0.003%
47	9.778	2700	2702	2704	rBV2	394	190	0.03%	0.004%
48	9.878	2731	2733	2734	rBV	337	147	0.02%	0.003%
49	10.254	2839	2850	2867	rBV	234582	365046	50.05%	6.941%
50	10.386	2886	2891	2894	rBV	356	233	0.03%	0.004%
51	10.717	2992	2994	2998	rBV	469	324	0.04%	0.006%
52	10.984	3075	3077	3081	rVB2	344	155	0.02%	0.003%
53	11.006	3081	3084	3085	rBV	344	192	0.03%	0.004%
54	11.196	3140	3143	3145	rBV2	341	214	0.03%	0.004%
55	11.289	3160	3172	3189	rBV	361954	563304	77.23%	10.711%
56	11.665	3277	3289	3311	rBV	346262	552334	75.72%	10.502%
57	12.119	3429	3430	3433	rVB2	382	158	0.02%	0.003%
58	12.325	3492	3494	3496	rBV2	464	231	0.03%	0.004%
59	12.595	3576	3578	3582	rBV2	336	253	0.03%	0.005%
60	12.659	3597	3598	3602	rVB2	267	113	0.02%	0.002%
61	12.913	3675	3677	3678	rBV	235	52	0.01%	0.001%
62	13.218	3770	3772	3776	rBV2	377	192	0.03%	0.004%
63	13.241	3777	3779	3781	rBV	348	174	0.02%	0.003%
64	13.334	3806	3808	3809	rBV	295	62	0.01%	0.001%
65	14.193	4073	4075	4080	rBV2	395	269	0.04%	0.005%
66	14.231	4083	4087	4090	rBV2	473	353	0.05%	0.007%
67	14.373	4128	4131	4132	rBV	416	241	0.03%	0.005%
68	14.910	4295	4298	4301	rBV2	492	368	0.05%	0.007%


Sum of corrected areas: 5259308

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022120\
Data File : VV014677.D
Acq On : 22 Feb 2020 01:02
Operator : SY/MD
Sample : L1608-08 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

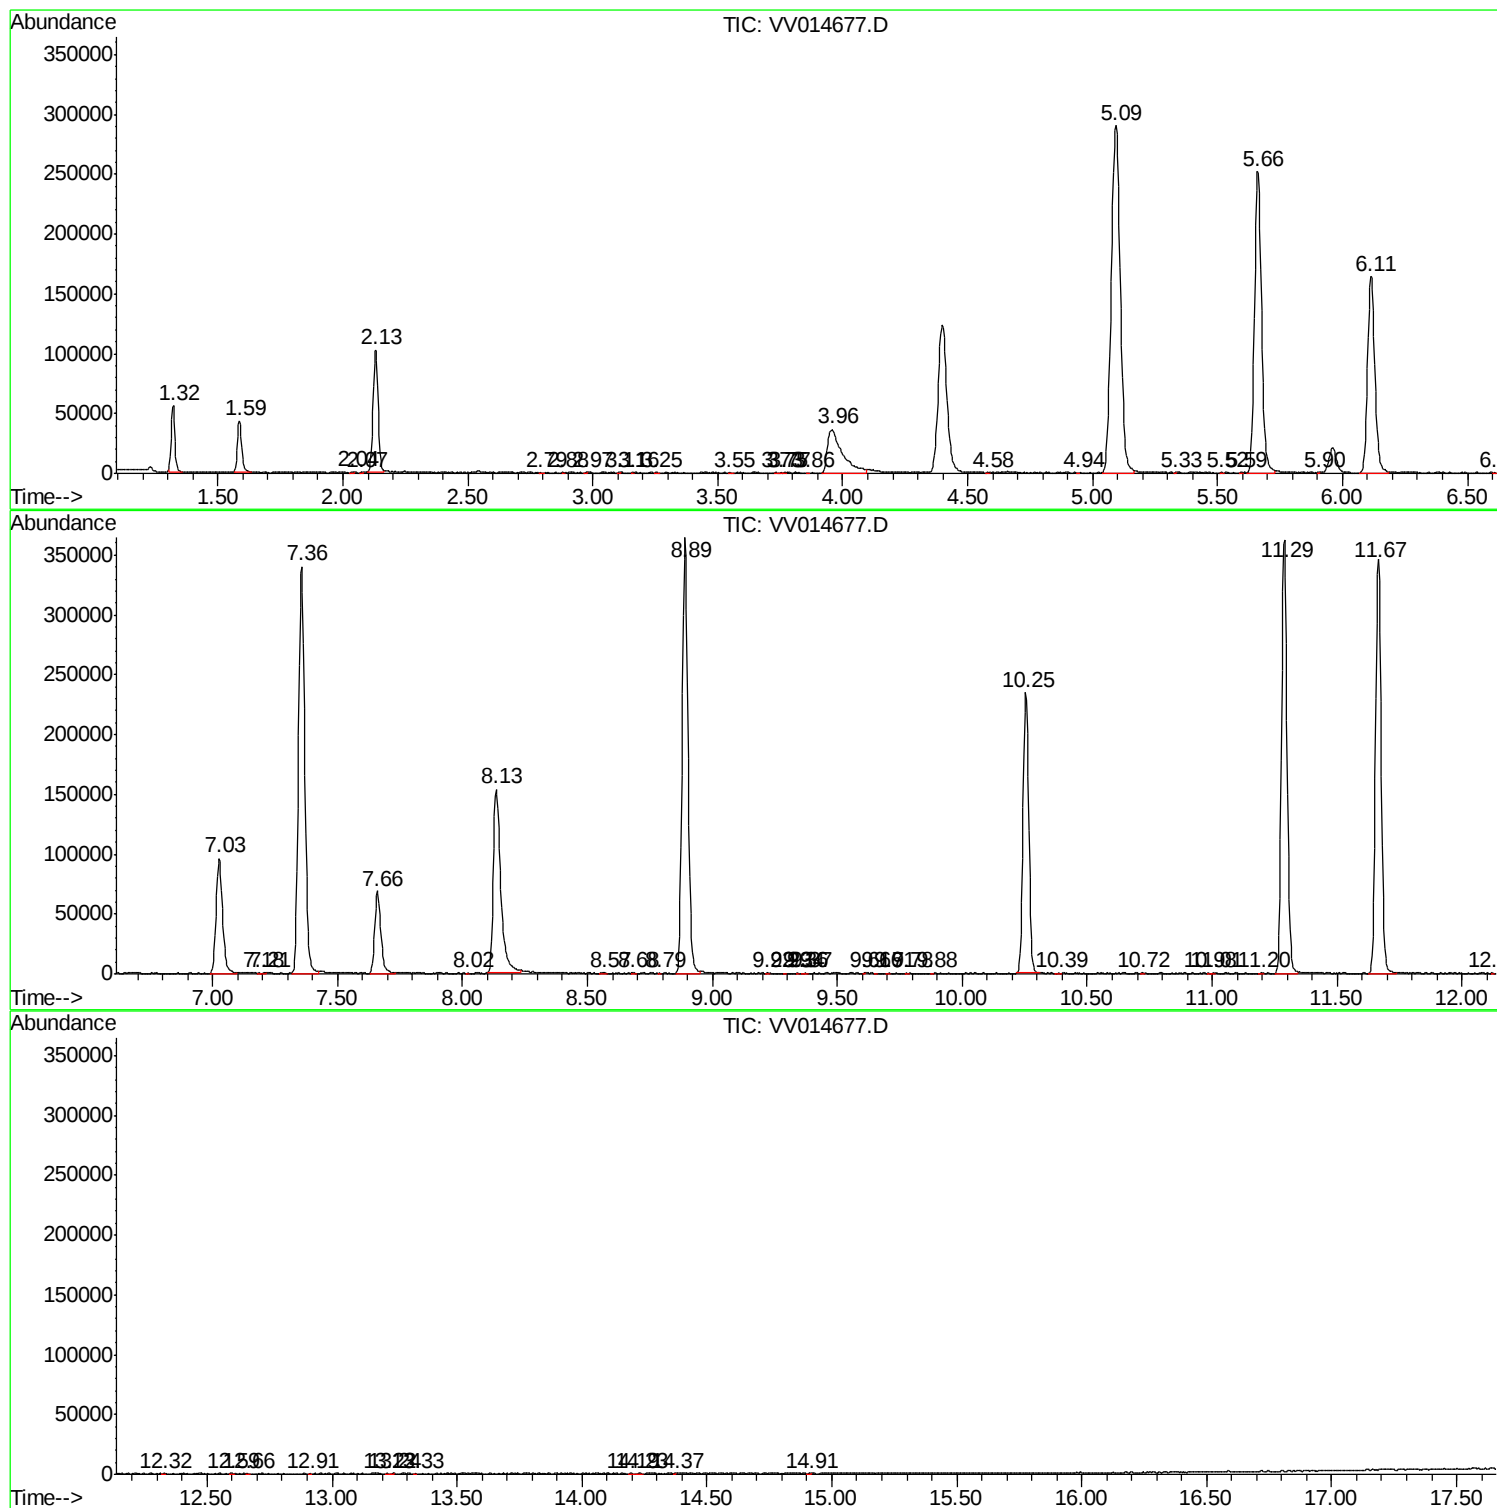

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022120\
Data File : VV014677.D
Acq On : 22 Feb 2020 01:02
Operator : SY/MD
Sample : L1608-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022120\
Data File : VV014677.D
Acq On : 22 Feb 2020 01:02
Operator : SY/MD
Sample : L1608-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc