

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\
 Data File : VV014684.D
 Acq On : 22 Feb 2020 03:45
 Operator : SY/MD
 Sample : L1608-12 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	66	71	84	rVB	54249	54707	7.52%	1.043%
2	1.586	147	154	166	rVB	42736	50508	6.94%	0.963%
3	2.007	283	285	288	rBV2	623	452	0.06%	0.009%
4	2.090	308	311	313	rBV3	456	338	0.05%	0.006%
5	2.129	313	323	336	rVV	101927	149406	20.53%	2.849%
6	3.148	639	640	643	rBV	403	141	0.02%	0.003%
7	3.216	660	661	663	rBV	221	98	0.01%	0.002%
8	3.402	716	719	722	rBV	595	336	0.05%	0.006%
9	3.566	768	770	771	rBV	399	142	0.02%	0.003%
10	3.843	854	856	857	rBV	375	189	0.03%	0.004%
11	3.904	871	875	877	rBV3	417	254	0.03%	0.005%
12	3.959	879	892	931	rBV	37200	155693	21.39%	2.969%
13	4.399	1011	1029	1049	rBV	123866	309298	42.50%	5.898%
14	4.708	1124	1125	1128	rBV2	241	67	0.01%	0.001%
15	4.721	1128	1129	1130	rBV	237	48	0.01%	0.001%
16	4.759	1139	1141	1145	rBV2	642	353	0.05%	0.007%
17	5.094	1228	1245	1267	rBV2	289293	727721	100.00%	13.876%
18	5.531	1379	1381	1383	rBV	374	112	0.02%	0.002%
19	5.659	1410	1421	1449	rVB	242625	480573	66.04%	9.163%
20	6.383	1642	1646	1648	rBV	354	215	0.03%	0.004%
21	6.441	1662	1664	1669	rBV2	373	343	0.05%	0.007%
22	6.653	1728	1730	1731	rBV	511	207	0.03%	0.004%
23	6.827	1782	1784	1787	rBV	235	163	0.02%	0.003%
24	6.888	1801	1803	1804	rBV	251	83	0.01%	0.002%
25	7.026	1834	1846	1868	rBV	94271	168222	23.12%	3.208%
26	7.357	1935	1949	1968	rBV	353004	612977	84.23%	11.688%
27	7.659	2033	2043	2059	rBV	66060	112418	15.45%	2.144%
28	7.929	2125	2127	2131	rBV	362	203	0.03%	0.004%
29	8.135	2181	2191	2228	rBV3	150794	321750	44.21%	6.135%
30	8.537	2314	2316	2318	rBV	352	192	0.03%	0.004%
31	8.608	2337	2338	2343	rBV3	308	207	0.03%	0.004%
32	8.740	2377	2379	2381	rBV2	492	261	0.04%	0.005%
33	8.891	2414	2426	2441	rBV	356279	579001	79.56%	11.040%
34	9.087	2482	2487	2490	rBV2	564	521	0.07%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022120\
 Data File : VV014684.D
 Acq On : 22 Feb 2020 03:45
 Operator : SY/MD
 Sample : L1608-12 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis

35	9.138	2500	2503	2505	rBV2	398	256	0.04%	0.005%
36	9.585	2640	2642	2643	rVB	348	85	0.01%	0.002%
37	9.952	2753	2756	2757	rBV	266	131	0.02%	0.002%
38	10.013	2773	2775	2777	rBV2	477	202	0.03%	0.004%
39	10.055	2786	2788	2791	rBV	273	111	0.02%	0.002%
40	10.254	2838	2850	2865	rBV	230376	359131	49.35%	6.848%
41	10.466	2914	2916	2919	rBV	314	161	0.02%	0.003%
42	10.537	2936	2938	2941	rVB2	403	183	0.03%	0.003%
43	10.971	3070	3073	3075	rBV2	550	262	0.04%	0.005%
44	11.071	3103	3104	3105	rVB	318	61	0.01%	0.001%
45	11.080	3105	3107	3110	rBV2	471	339	0.05%	0.006%
46	11.286	3160	3171	3193	rBV	368697	574870	79.00%	10.961%
47	11.666	3277	3289	3309	rBV	364737	580010	79.70%	11.059%
48	11.897	3359	3361	3362	rVB2	348	95	0.01%	0.002%
49	11.968	3381	3383	3384	rBV	343	111	0.02%	0.002%
50	13.145	3747	3749	3750	rBV	307	146	0.02%	0.003%
51	13.714	3922	3926	3933	rBV	552	874	0.12%	0.017%
52	13.826	3960	3961	3967	rBV	327	279	0.04%	0.005%


Sum of corrected areas: 5244506

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022120\
Data File : VV014684.D
Acq On : 22 Feb 2020 03:45
Operator : SY/MD
Sample : L1608-12 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

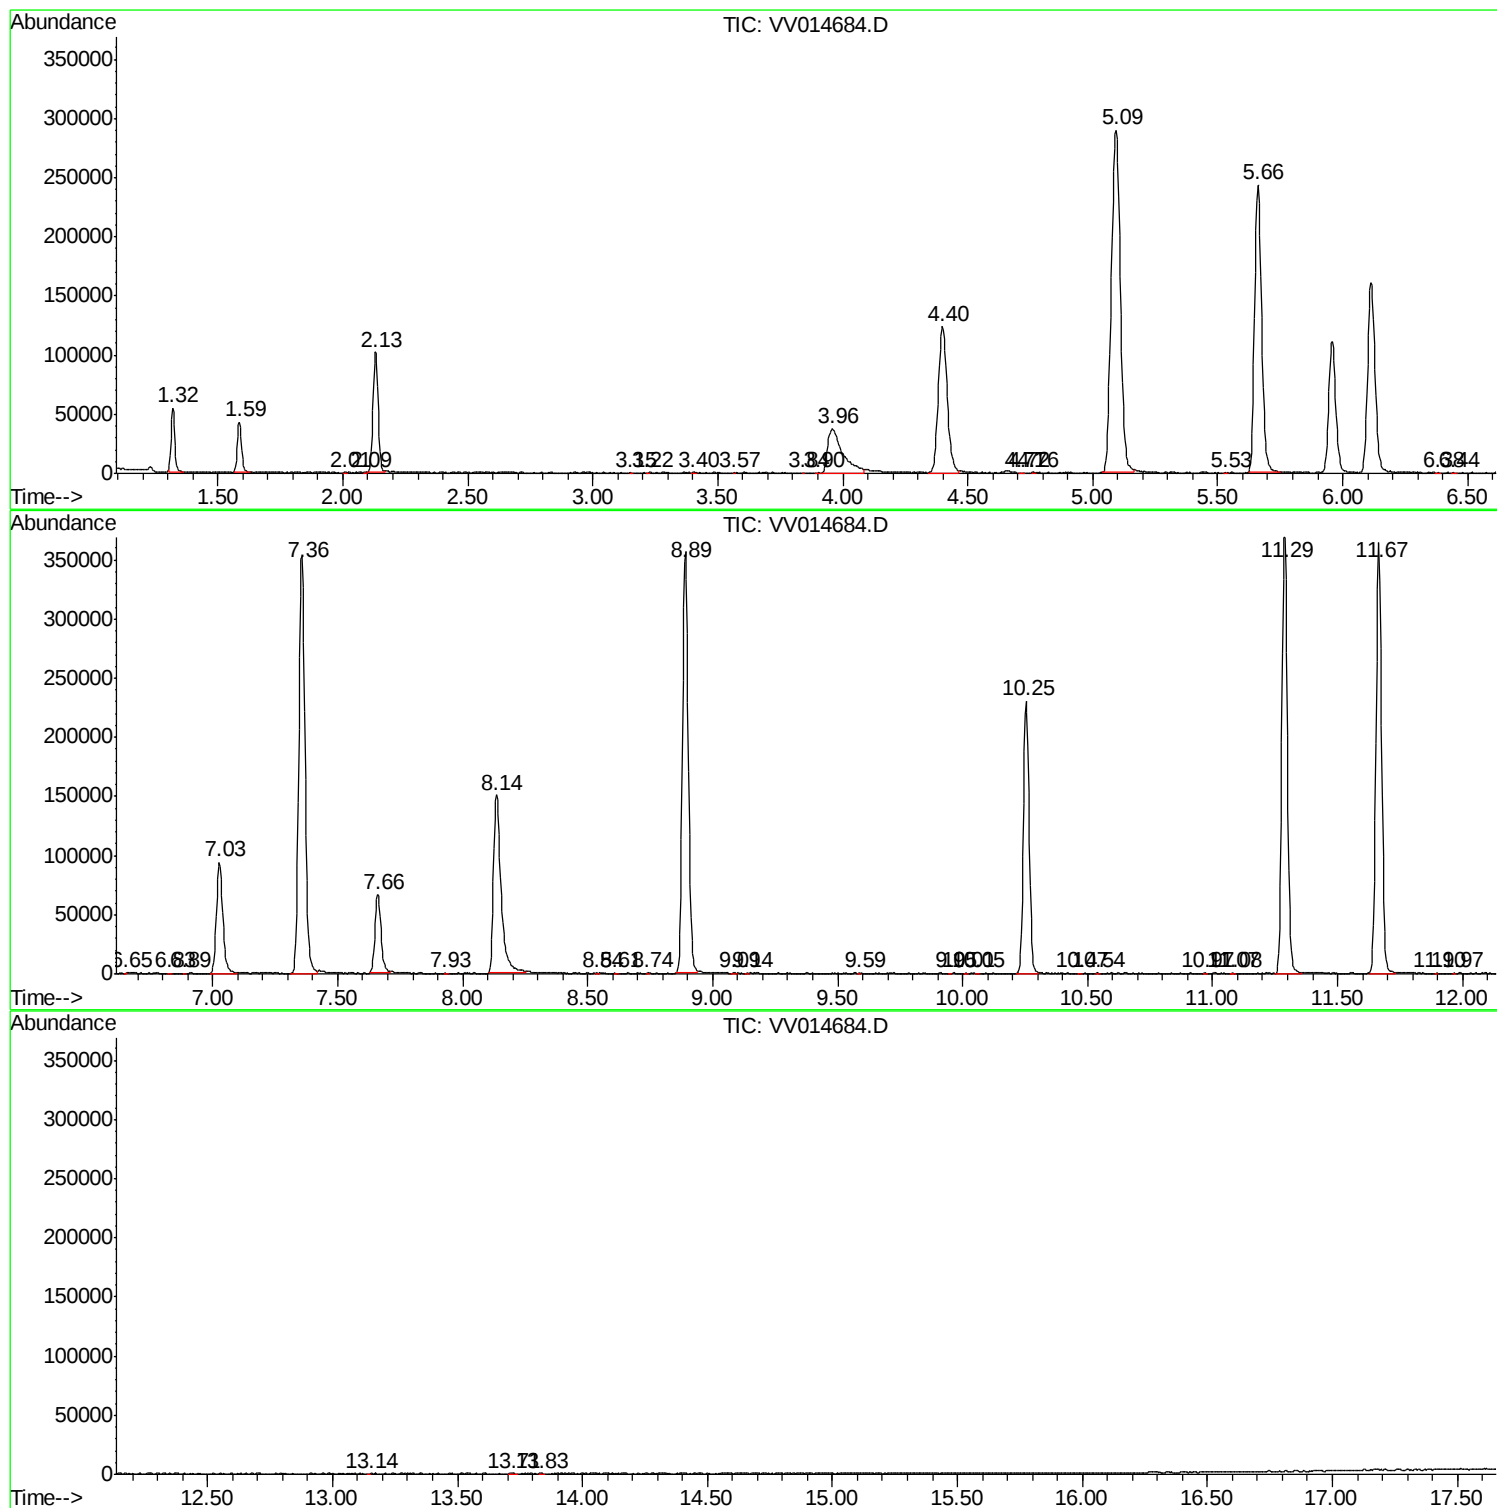

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022120\
Data File : VV014684.D
Acq On : 22 Feb 2020 03:45
Operator : SY/MD
Sample : L1608-12 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022120\
Data File : VV014684.D
Acq On : 22 Feb 2020 03:45
Operator : SY/MD
Sample : L1608-12 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc