


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV022120\
 Data File : VV014644.D
 Acq On : 21 Feb 2020 09:45
 Operator : SY/MD
 Sample : BFB94
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB94

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis
 Last Update : Mon Feb 24 04:25:56 2020

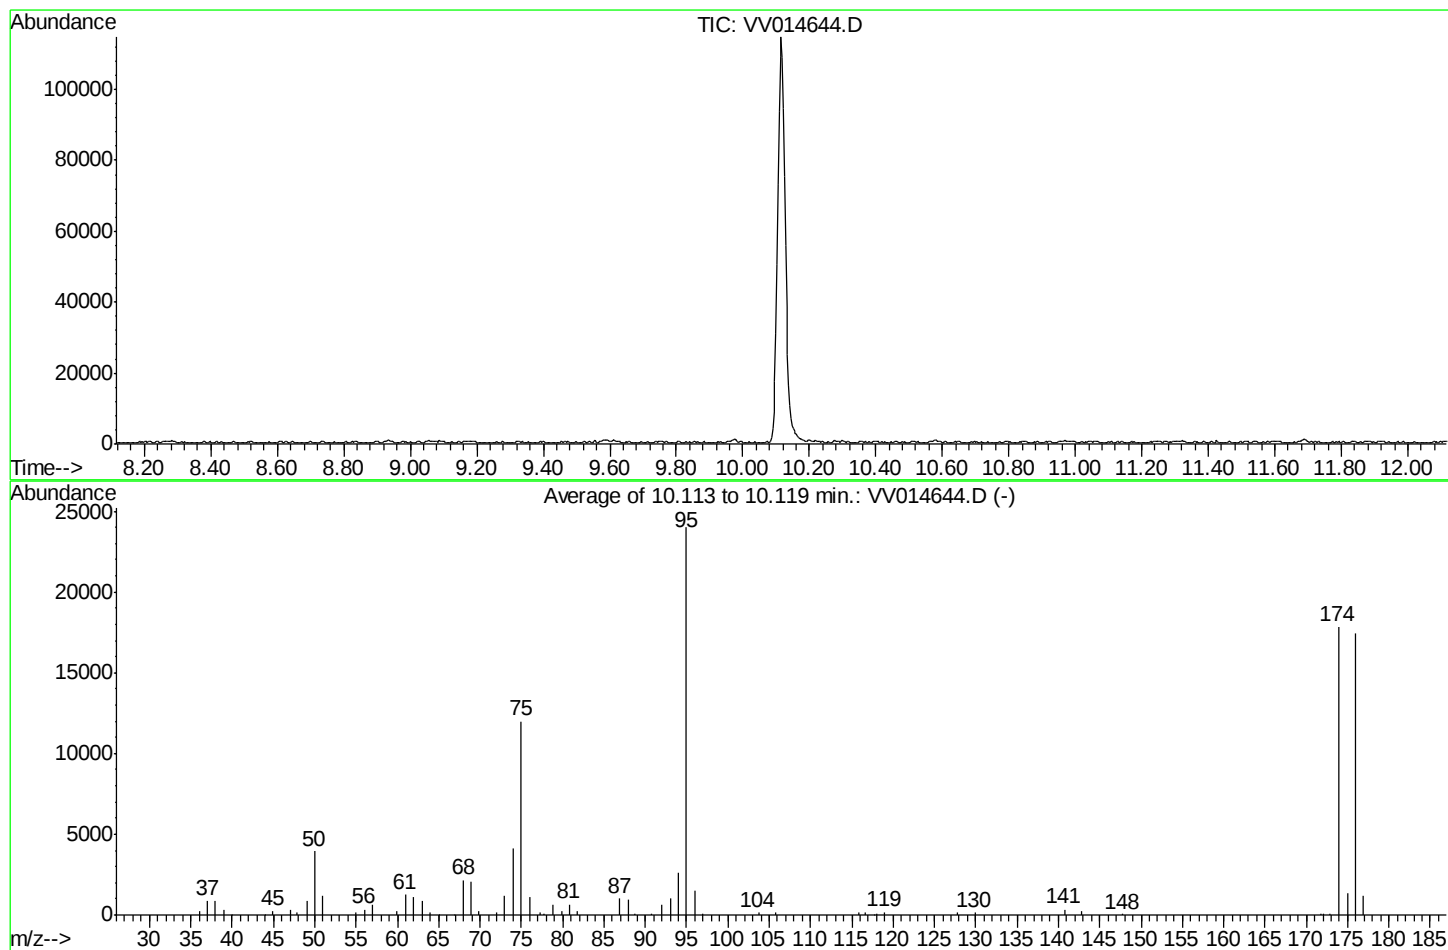

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	3932	PASS
75	95	30	80	49.9	11979	PASS
95	95	100	100	100.0	24000	PASS
96	95	5	9	6.3	1511	PASS
173	174	0.00	2	0.5	87	PASS
174	95	50	120	74.3	17837	PASS
175	174	5	9	7.6	1358	PASS
176	174	95	101	97.6	17408	PASS
177	176	5	9	6.6	1157	PASS

m/z	Abundance
36.00	232.0
37.00	904.0
38.00	933.0
39.00	362.0
40.00	221.0
44.00	272.0
45.00	270.0
47.00	382.0
47.90	166.0
49.00	963.0
50.00	4048.0
50.90	1197.0
54.90	170.0
56.00	359.0
57.00	587.0
59.90	253.0
61.00	1280.0
62.00	1222.0
63.00	832.0
64.00	132.0
68.00	2116.0
68.90	2035.0
69.90	273.0
71.90	150.0
73.00	1291.0
74.00	4215.0
75.00	11992.0
76.00	1088.0
77.20	160.0
78.80	634.0
79.90	225.0
80.80	645.0
81.80	221.0
86.90	1089.0
87.90	1099.0
90.80	110.0
92.00	659.0
93.00	966.0
94.00	2626.0
95.00	23864.0
96.00	1500.0
97.00	113.0
103.70	122.0
105.70	117.0
115.90	145.0
116.60	139.0
117.70	107.0
119.00	171.0
127.70	149.0
129.90	145.0
140.70	273.0
142.80	274.0
171.80	165.0
173.90	16808.0
174.90	1330.0
175.90	16584.0
177.00	1095.0

Instrument :
MSVOA_V
ClientSampleId :
BFB94

m/z	Abundance
36.00	217.0
37.00	927.0
38.00	885.0
39.00	300.0
40.00	192.0
44.00	259.0
45.00	264.0
47.00	369.0
47.80	171.0
49.00	905.0
50.00	4031.0
50.90	1183.0
54.90	145.0
56.00	340.0
57.00	592.0
59.90	233.0
61.00	1306.0
62.00	1212.0
63.00	890.0
63.90	133.0
68.00	2203.0
68.90	2113.0
69.90	271.0
72.00	165.0
73.00	1260.0
74.00	4257.0
75.00	12523.0
76.00	1125.0
77.20	184.0
77.70	105.0
78.80	643.0
80.00	256.0
80.80	660.0
81.80	212.0
86.90	1051.0
87.90	1013.0
88.70	117.0
90.80	108.0
92.00	640.0
93.00	1077.0
94.00	2707.0
95.00	24904.0
96.00	1547.0
97.00	122.0
103.70	137.0
105.70	128.0
115.80	143.0
116.60	129.0
118.10	111.0
118.90	183.0
127.70	146.0
129.90	153.0
140.70	355.0
142.80	283.0
147.80	104.0
171.80	154.0
173.90	18488.0
175.00	1383.0
176.00	17944.0
176.90	1166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB94

m/z	Abundance
36.00	200.0
37.00	866.0
37.90	718.0
39.00	280.0
39.90	150.0
44.00	238.0
44.90	225.0
47.00	302.0
47.80	161.0
49.00	869.0
50.00	3717.0
50.90	1094.0
55.00	117.0
56.00	289.0
57.10	616.0
60.00	222.0
60.90	1130.0
62.00	981.0
62.90	827.0
63.90	123.0
65.10	126.0
66.90	118.0
68.00	2168.0
68.90	2039.0
69.90	213.0
72.00	194.0
73.00	1100.0
74.00	3800.0
75.00	11424.0
76.00	1037.0
77.20	158.0
77.80	123.0
78.90	643.0
80.00	237.0
80.80	655.0
81.80	192.0
87.00	906.0
87.90	815.0
88.70	118.0
91.90	641.0
93.00	1056.0
93.90	2490.0
95.00	23232.0
96.10	1487.0
97.00	114.0
103.80	141.0
105.70	129.0
115.70	150.0
116.70	112.0
118.00	107.0
118.90	201.0
127.80	128.0
129.90	133.0
140.80	407.0
142.90	277.0
147.80	107.0
172.00	167.0
172.80	263.0
173.90	18216.0
175.00	1362.0
176.00	17696.0
176.90	1211.0

Instrument :
MSVOA_V
ClientSampleId :
BFB94

Scan 2795 (10.077 min): VV014644.D
BFB94

m/z	Abundance
40.00	155.0
43.90	255.0

Instrument :
MSVOA_V
ClientSampleId :
BFB94