




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
 Data File : VV034307.D
 Acq On : 21 Feb 2024 10:02
 Operator : SY/MD
 Sample : VV0221WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK221

Manual IntegrationsAPPROVED

Quant Time: Feb 22 00:19:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 22 00:18:57 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/22/2024
 Supervised By :Mahesh Dadoda 02/22/2024

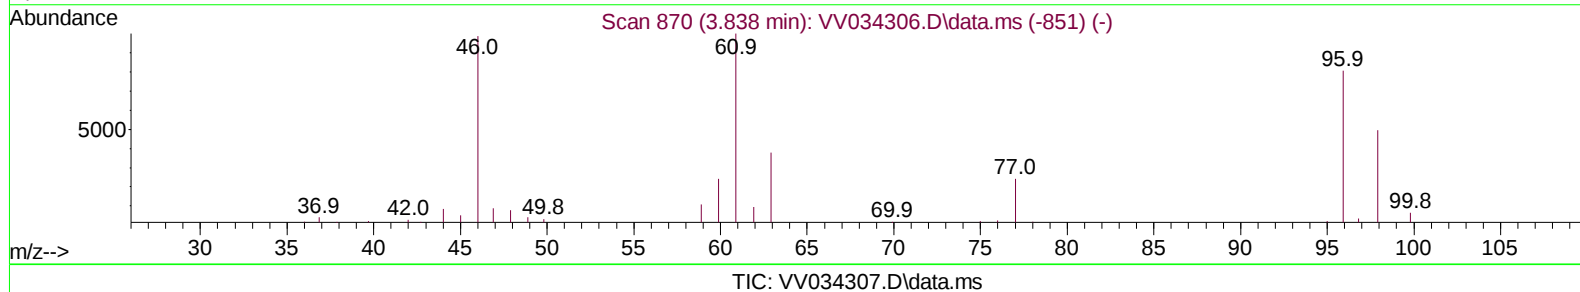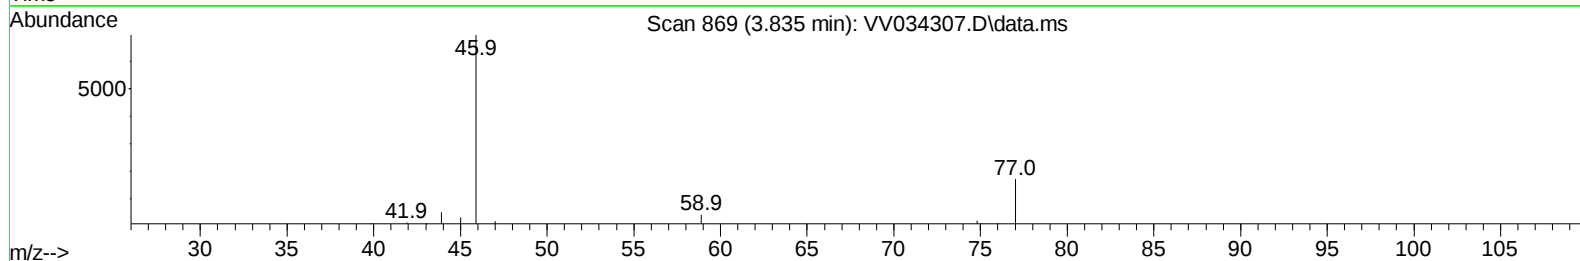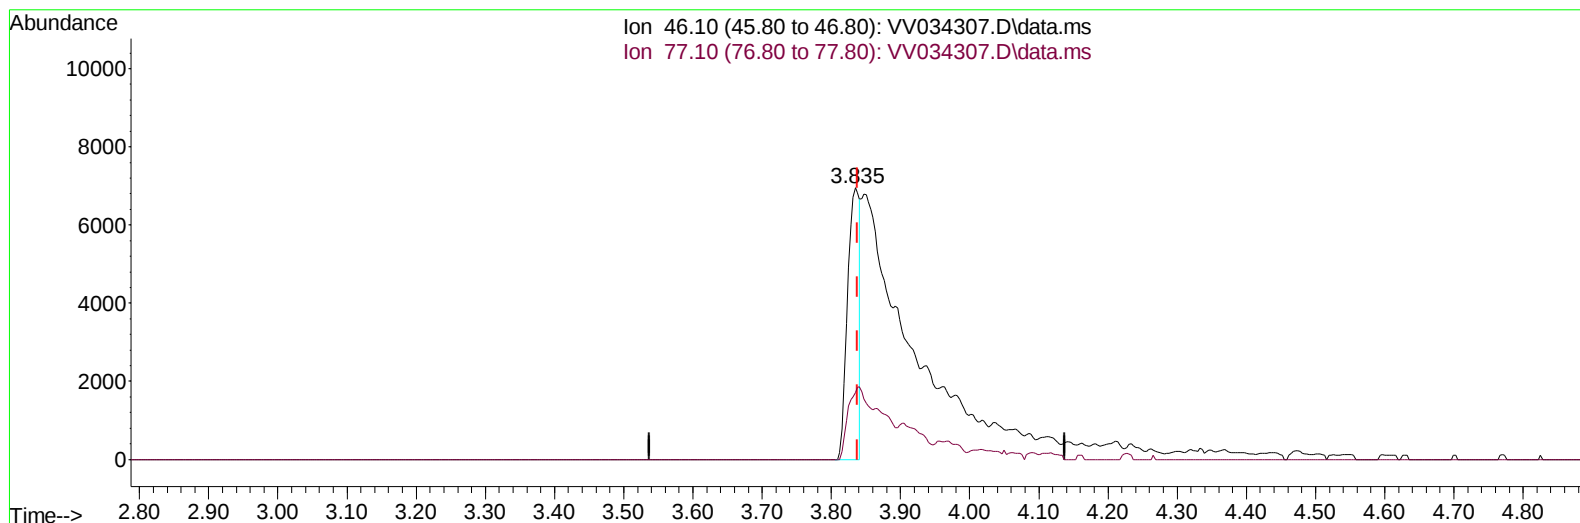

(20) 2-Butanone-d5 (S)

3.835min (-0.003) 8.55 ug/L

response 8578

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.80	45.76#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
 Data File : VV034307.D
 Acq On : 21 Feb 2024 10:02
 Operator : SY/MD
 Sample : VV0221WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK221

Manual IntegrationsAPPROVED

Quant Time: Feb 22 00:19:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 22 00:18:57 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/22/2024
 Supervised By :Mahesh Dadoda 02/22/2024

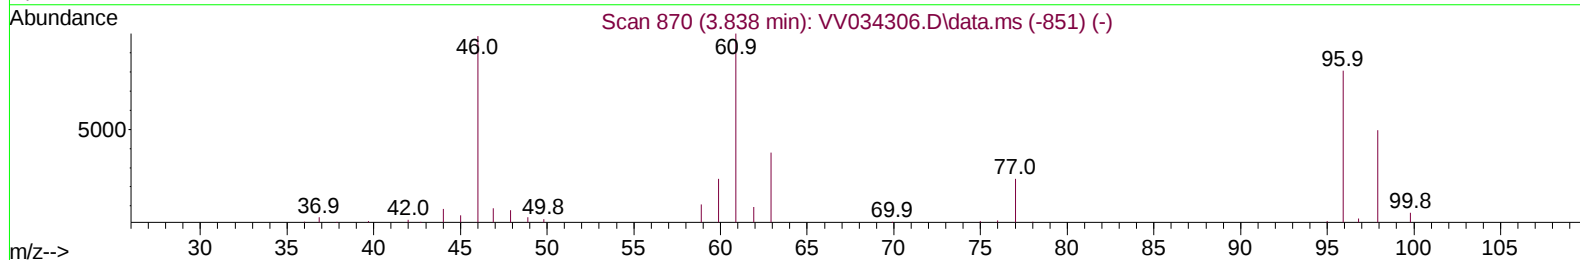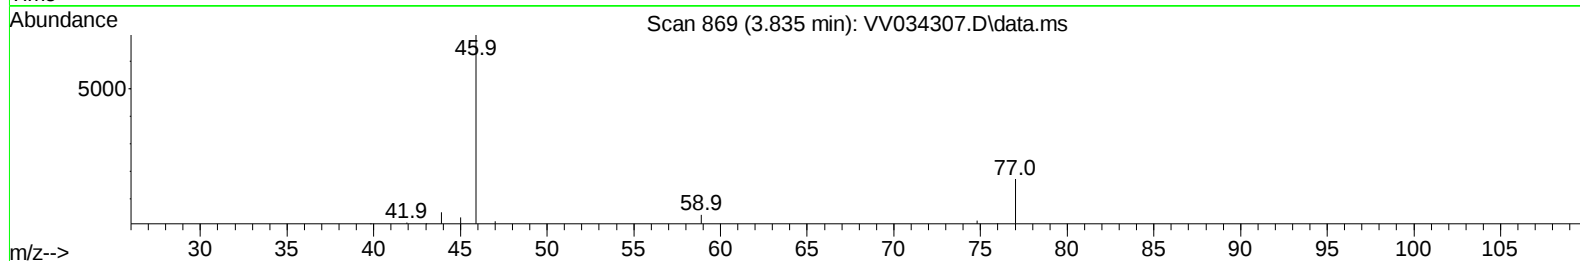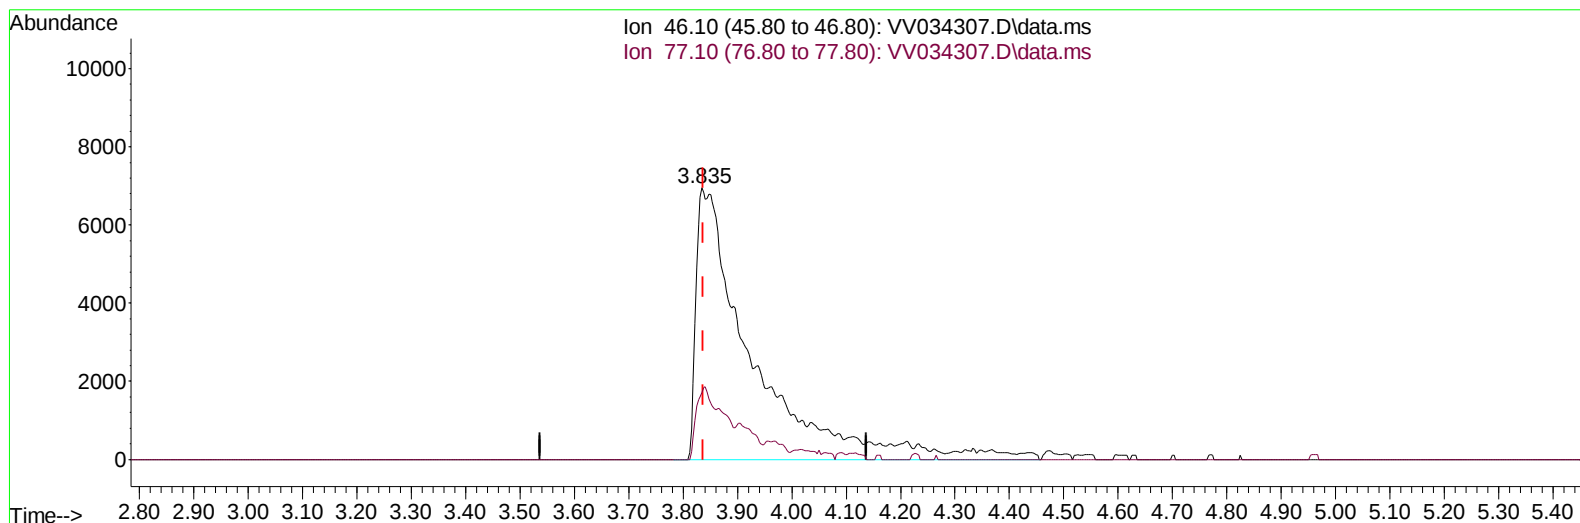

TIC: VV034307.D\data.ms

(20) 2-Butanone-d5 (S)

3.835min (-0.003) 49.51 ug/L m

response 49691

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.80	7.90#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
 Data File : VV034307.D
 Acq On : 21 Feb 2024 10:02
 Operator : SY/MD
 Sample : VV0221WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK221

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/22/2024
 Supervised By :Mahesh Dadoda 02/22/2024

Quant Time: Feb 22 00:19:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 22 00:18:57 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		77162	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		71523	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		33826	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		22818	3.818	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.400%	
7) Chloroethane-d5	1.532	69		21648	4.136	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.800%	
11) 1,1-Dichloroethene-d2	2.060	65		11808	4.097	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.000%	
20) 2-Butanone-d5	3.835	46		49691m	49.510	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.020%	
24) Chloroform-d	4.249	84		50746	4.673	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4	4.944	65		24933	4.913	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%	
32) Benzene-d6	4.960	84		92905	4.329	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.600%	
36) 1,2-Dichloropropane-d6	5.989	67		26263	4.378	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.600%	
41) Toluene-d8	7.243	98		83687	4.243	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.800%	
43) trans-1,3-Dichloroprop...	7.561	79		7727	3.412	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.200%	
46) 2-Hexanone-d5	8.030	63		32414	40.089	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.180%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84		15756	4.333	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.600%	
66) 1,2-Dichlorobenzene-d4	11.561	152		29074	4.726	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.600%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
Data File : VV034307.D
Acq On : 21 Feb 2024 10:02
Operator : SY/MD
Sample : VV0221WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK221

Manual IntegrationsAPPROVED

Quant Time: Feb 22 00:19:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 22 00:18:57 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/22/2024
Supervised By :Mahesh Dadoda 02/22/2024

