




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
Data File : VV034324.D
Acq On : 21 Feb 2024 17:09
Operator : SY/MD
Sample : P1498-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/22/2024
Supervised By :Mahesh Dadoda 02/22/2024

Quant Time: Feb 22 00:23:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 22 00:18:57 2024
Response via : Initial Calibration

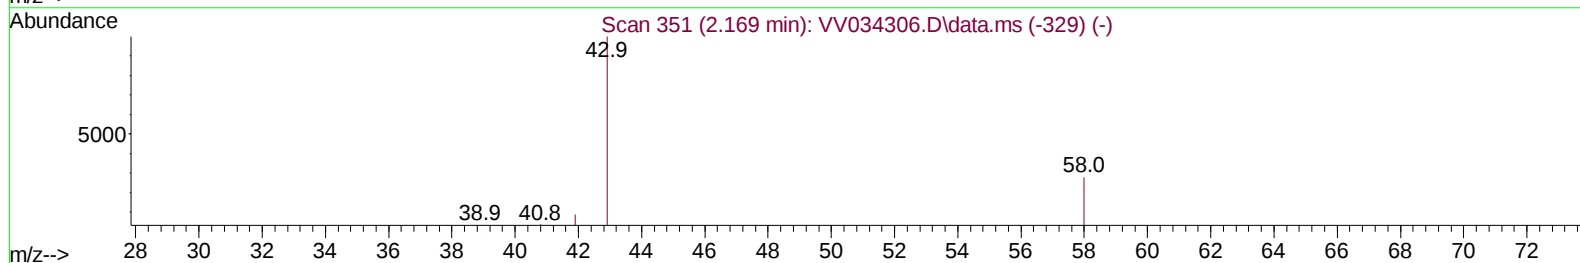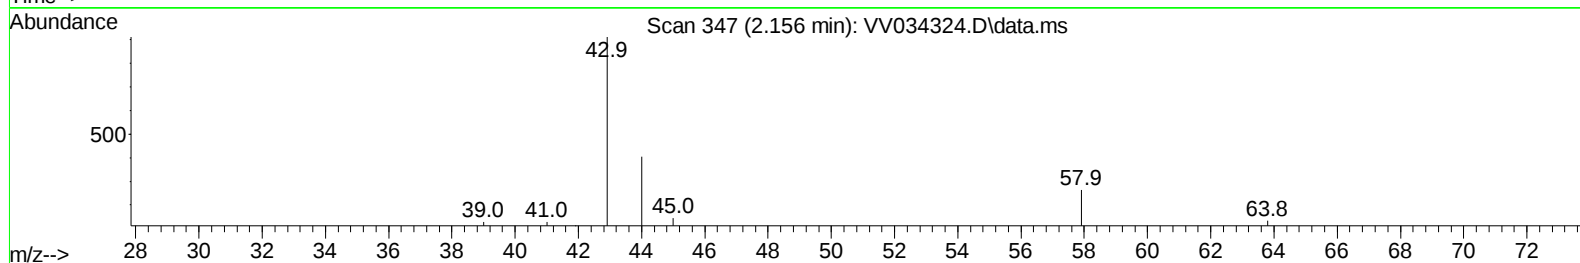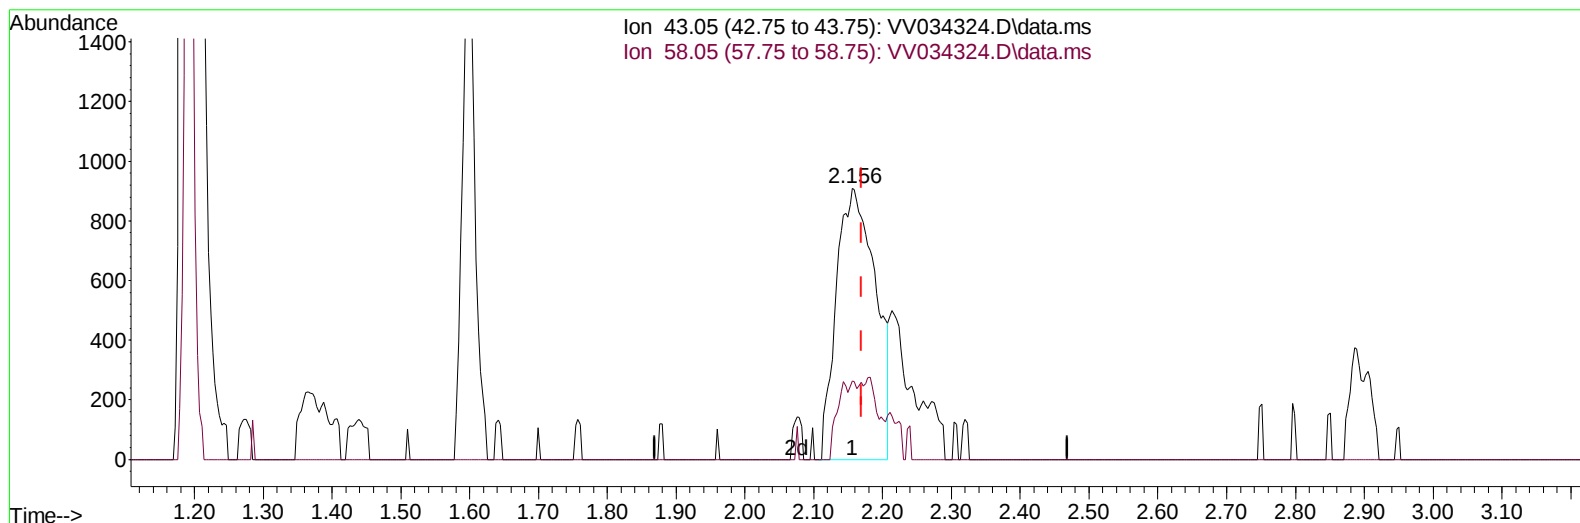

TIC: VV034324.D\data.ms

(13) Acetone (T)

2.156min (-0.013) 4.35 ug/L

response 3590

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	6.90	1.23
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
Data File : VV034324.D
Acq On : 21 Feb 2024 17:09
Operator : SY/MD
Sample : P1498-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/22/2024
Supervised By :Mahesh Dadoda 02/22/2024

Quant Time: Feb 22 00:23:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 22 00:18:57 2024
Response via : Initial Calibration

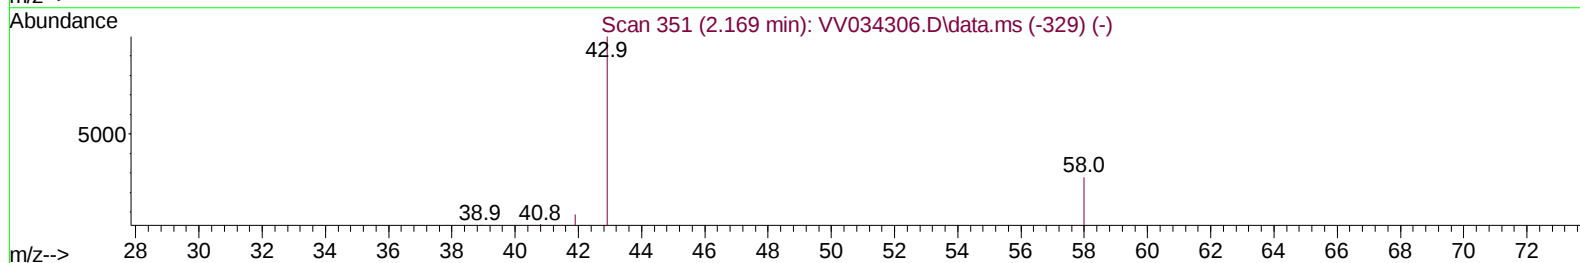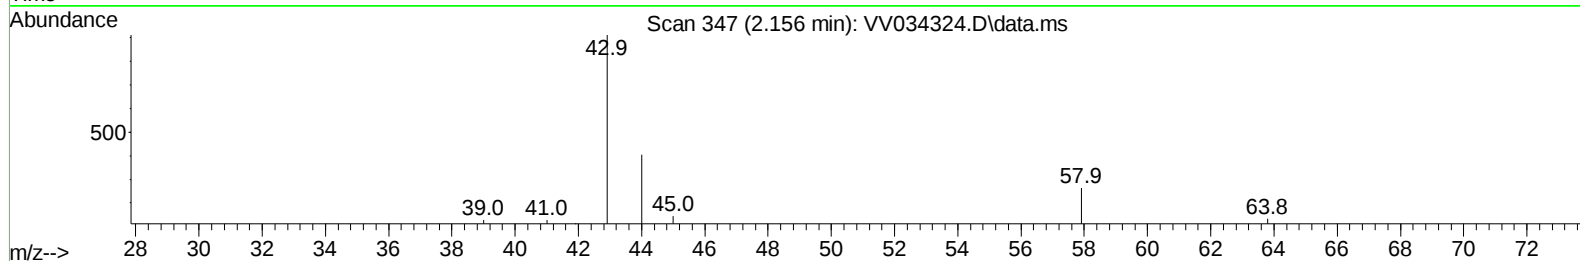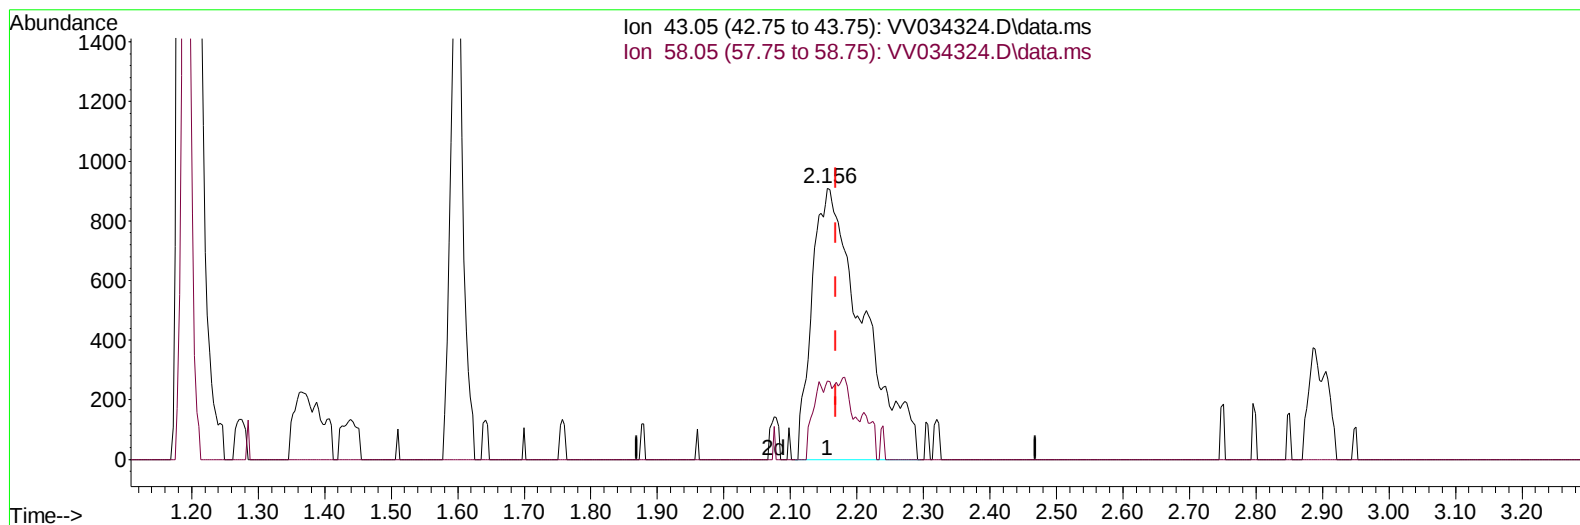

TIC: VV034324.D\data.ms

(13) Acetone (T)

2.156min (-0.013) 5.85 ug/L m

response 4827

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	6.90	0.91
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
 Data File : VV034324.D
 Acq On : 21 Feb 2024 17:09
 Operator : SY/MD
 Sample : P1498-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG2

Manual IntegrationsAPPROVED

Quant Time: Feb 22 00:23:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 22 00:18:57 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/22/2024
 Supervised By :Mahesh Dadoda 02/22/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		83595	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		75282	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		35803	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		19732	3.048	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	61.000%		
7) Chloroethane-d5	1.535	69		19513	3.441	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	68.800%		
11) 1,1-Dichloroethene-d2	2.059	65		10527	3.372	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	67.400%		
20) 2-Butanone-d5	3.831	46		50237	46.202	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	92.400%		
24) Chloroform-d	4.249	84		48817	4.150	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	83.000%		
26) 1,2-Dichloroethane-d4	4.947	65		25411	4.622	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	92.400%		
32) Benzene-d6	4.960	84		89974	3.984	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	79.600%		
36) 1,2-Dichloropropane-d6	5.989	67		26262	4.160	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	83.200%		
41) Toluene-d8	7.246	98		81116	3.908	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	78.200%		
43) trans-1,3-Dichloroprop...	7.561	79		7938	3.330	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	66.600%		
46) 2-Hexanone-d5	8.030	63		39243	46.112	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	92.220%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84		18099	4.729	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	94.600%		
66) 1,2-Dichlorobenzene-d4	11.561	152		29923	4.596	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	92.000%		
Target Compounds							
13) Acetone	2.156	43		4827m	5.852	ug/L	
42) Toluene	7.329	91		3059	0.127	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
Data File : VV034324.D
Acq On : 21 Feb 2024 17:09
Operator : SY/MD
Sample : P1498-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0AG2

Manual IntegrationsAPPROVED

Quant Time: Feb 22 00:23:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 22 00:18:57 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/22/2024
Supervised By :Mahesh Dadoda 02/22/2024

