

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
 Data File : VV034324.D
 Acq On : 21 Feb 2024 17:09
 Operator : SY/MD
 Sample : P1498-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 02/22/2024
 Supervised By :Mahesh Dadoda 02/22/2024

Quant Time: Feb 22 00:23:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 22 00:18:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	83595	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	75282	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	35803	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	19732	3.048	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	61.000%	
7) Chloroethane-d5	1.535	69	19513	3.441	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	68.800%	
11) 1,1-Dichloroethene-d2	2.059	65	10527	3.372	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.400%	
20) 2-Butanone-d5	3.831	46	50237	46.202	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	92.400%	
24) Chloroform-d	4.249	84	48817	4.150	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.000%	
26) 1,2-Dichloroethane-d4	4.947	65	25411	4.622	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.400%	
32) Benzene-d6	4.960	84	89974	3.984	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	79.600%	
36) 1,2-Dichloropropane-d6	5.989	67	26262	4.160	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	83.200%	
41) Toluene-d8	7.246	98	81116	3.908	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	78.200%	
43) trans-1,3-Dichloroprop...	7.561	79	7938	3.330	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	66.600%	
46) 2-Hexanone-d5	8.030	63	39243	46.112	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	92.220%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	18099	4.729	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.600%	
66) 1,2-Dichlorobenzene-d4	11.561	152	29923	4.596	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.000%	
Target Compounds					Qvalue	
13) Acetone	2.156	43	4827m	5.852	ug/L	
42) Toluene	7.329	91	3059	0.127	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
Data File : VV034324.D
Acq On : 21 Feb 2024 17:09
Operator : SY/MD
Sample : P1498-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0AG2

Quant Time: Feb 22 00:23:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 22 00:18:57 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/22/2024
Supervised By :Mahesh Dadoda 02/22/2024

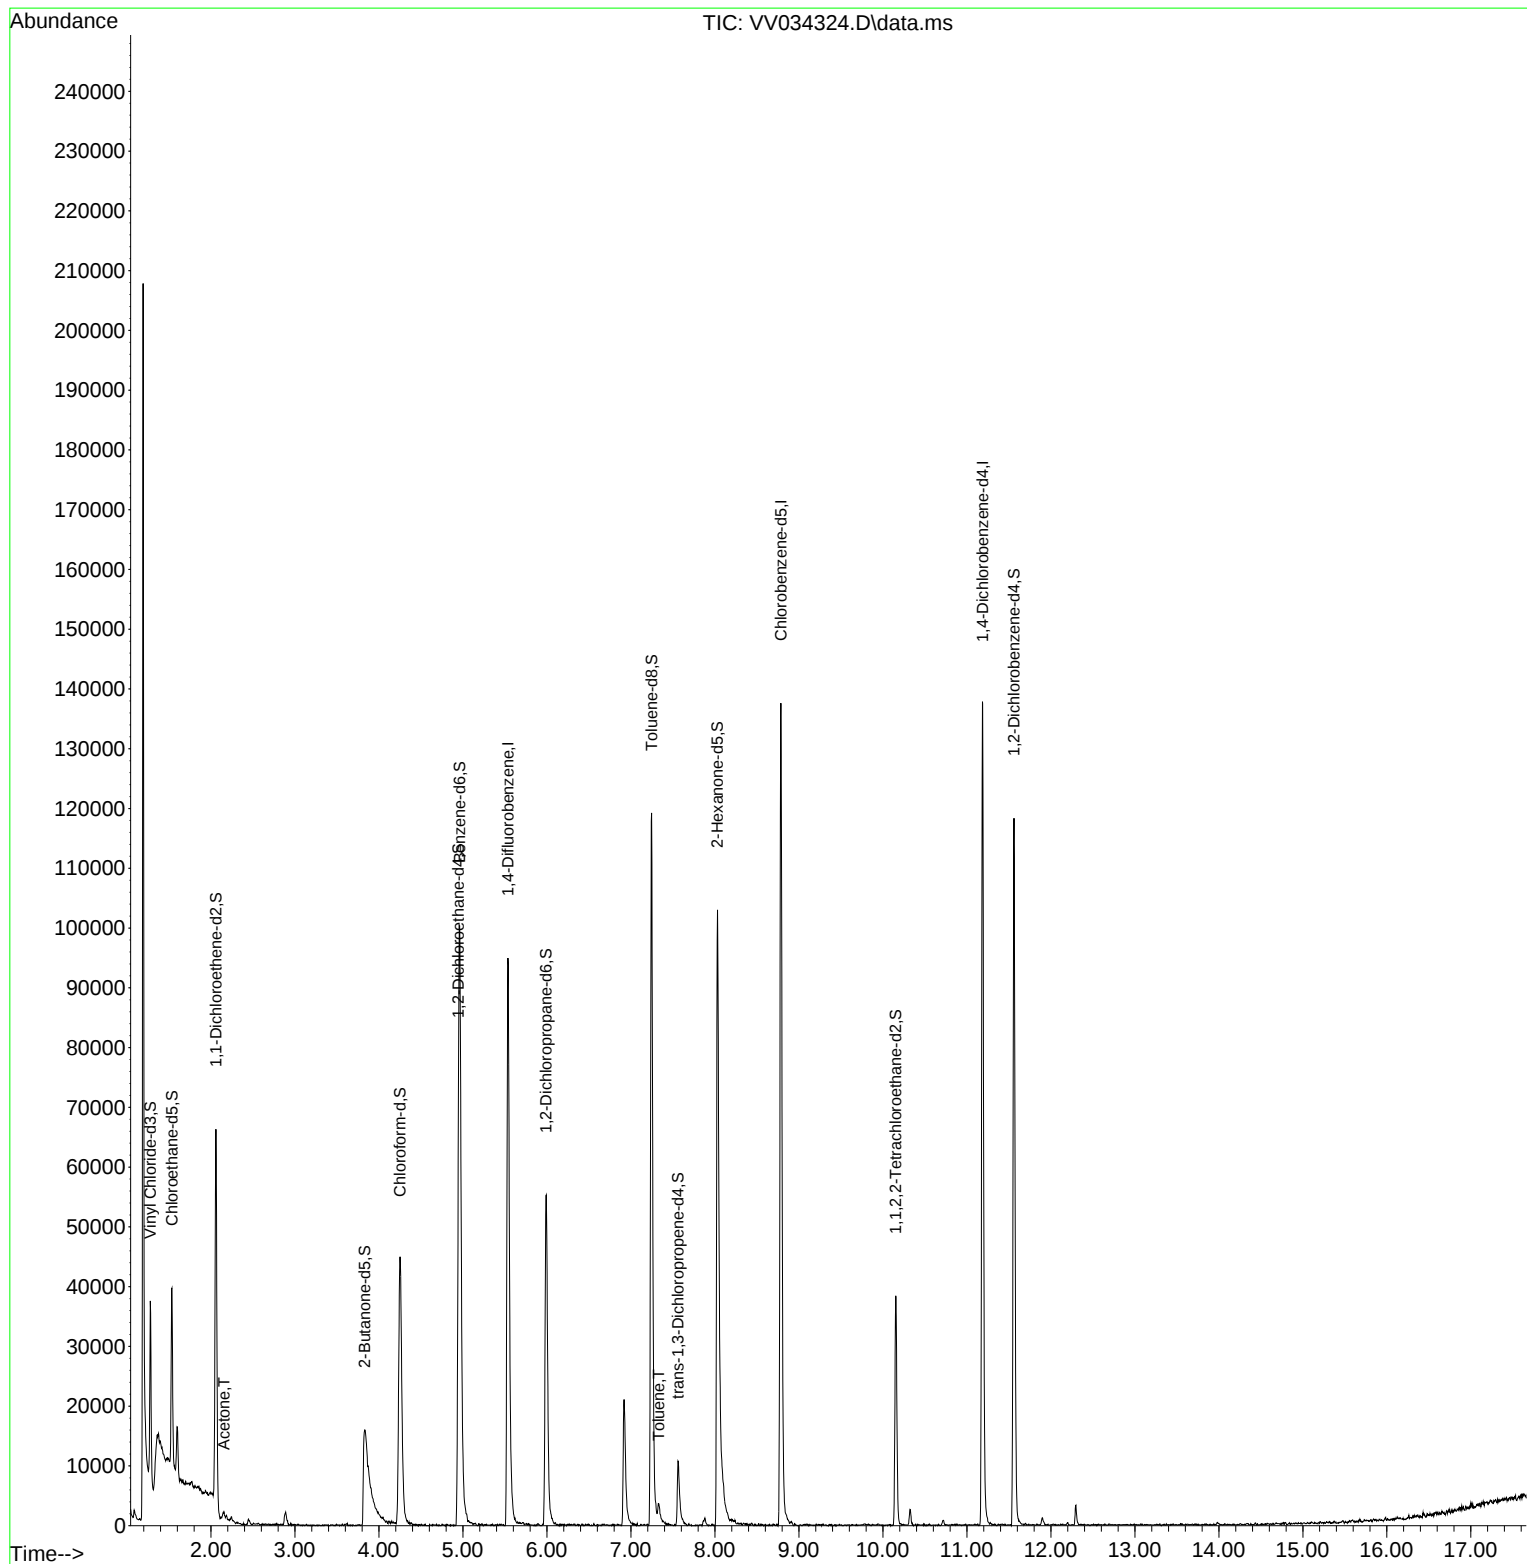

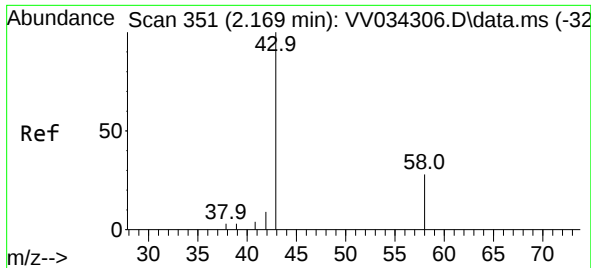

#13
Acetone
Concen: 5.852 ug/L m
RT: 2.156 min Scan# 347
Delta R.T. -0.013 min
Lab File: VV034324.D
Acq: 21 Feb 2024 17:09




Instrument :
MSVOA_V
ClientSampleId :
C0AG2

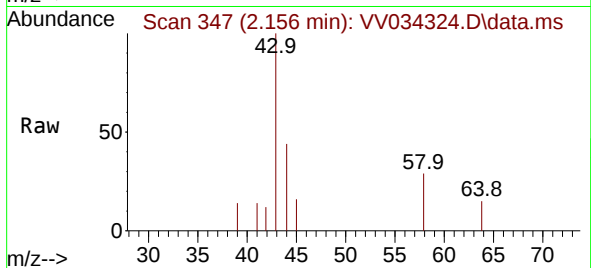


Tgt Ion: 43 Resp: 482
Ion Ratio Lower Upper
43 100
58 0.9 0.0 13.8

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 02/22/2024
Supervised By :Mahesh Dadoda 02/22/2024

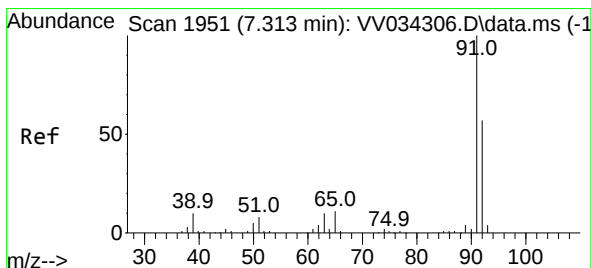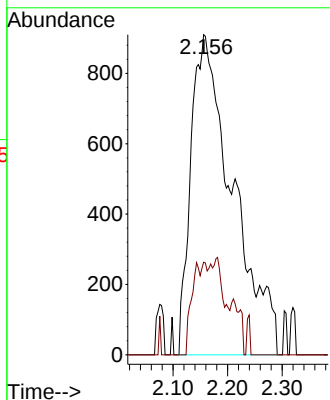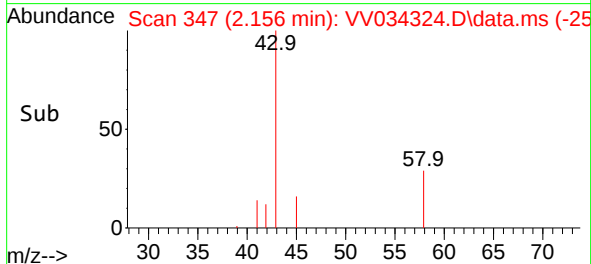

#42
Toluene
Concen: 0.127 ug/L
RT: 7.329 min Scan# 1956
Delta R.T. 0.016 min
Lab File: VV034324.D
Acq: 21 Feb 2024 17:09

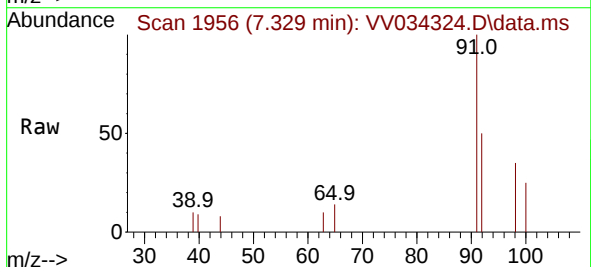

Tgt Ion: 91 Resp: 3059
Ion Ratio Lower Upper
91 100
92 49.6 42.1 78.3

