

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022124\
 Data File : VW034325.D
 Acq On : 21 Feb 2024 17:33
 Operator : SY/MD
 Sample : P1498-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH3

Quant Time: Feb 22 00:23:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 22 00:18:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	60387	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	56316	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	26364	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	15087	3.226	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	64.600%	
7) Chloroethane-d5	1.535	69	14702	3.589	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	71.800%	
11) 1,1-Dichloroethene-d2	2.060	65	8246	3.656	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	73.200%	
20) 2-Butanone-d5	3.818	46	49598	63.145	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	126.300%	
24) Chloroform-d	4.256	84	37189	4.376	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.600%	
26) 1,2-Dichloroethane-d4	4.947	65	21906	5.516	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	110.400%	
32) Benzene-d6	4.963	84	66521	3.937	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	78.800%	
36) 1,2-Dichloropropane-d6	5.992	67	20313	4.301	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	86.000%	
41) Toluene-d8	7.246	98	59410	3.826	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	76.600%	
43) trans-1,3-Dichloroprop...	7.564	79	7019	3.936	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.800%	
46) 2-Hexanone-d5	8.027	63	40771	64.041	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	128.080%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	17231	6.018	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	120.400%#	
66) 1,2-Dichlorobenzene-d4	11.561	152	22975	4.792	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	95.800%	
Target Compounds						
13) Acetone	2.146	43	4590	7.703	ug/L	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
Data File : VV034325.D
Acq On : 21 Feb 2024 17:33
Operator : SY/MD
Sample : P1498-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH3

Quant Time: Feb 22 00:23:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 22 00:18:57 2024
Response via : Initial Calibration

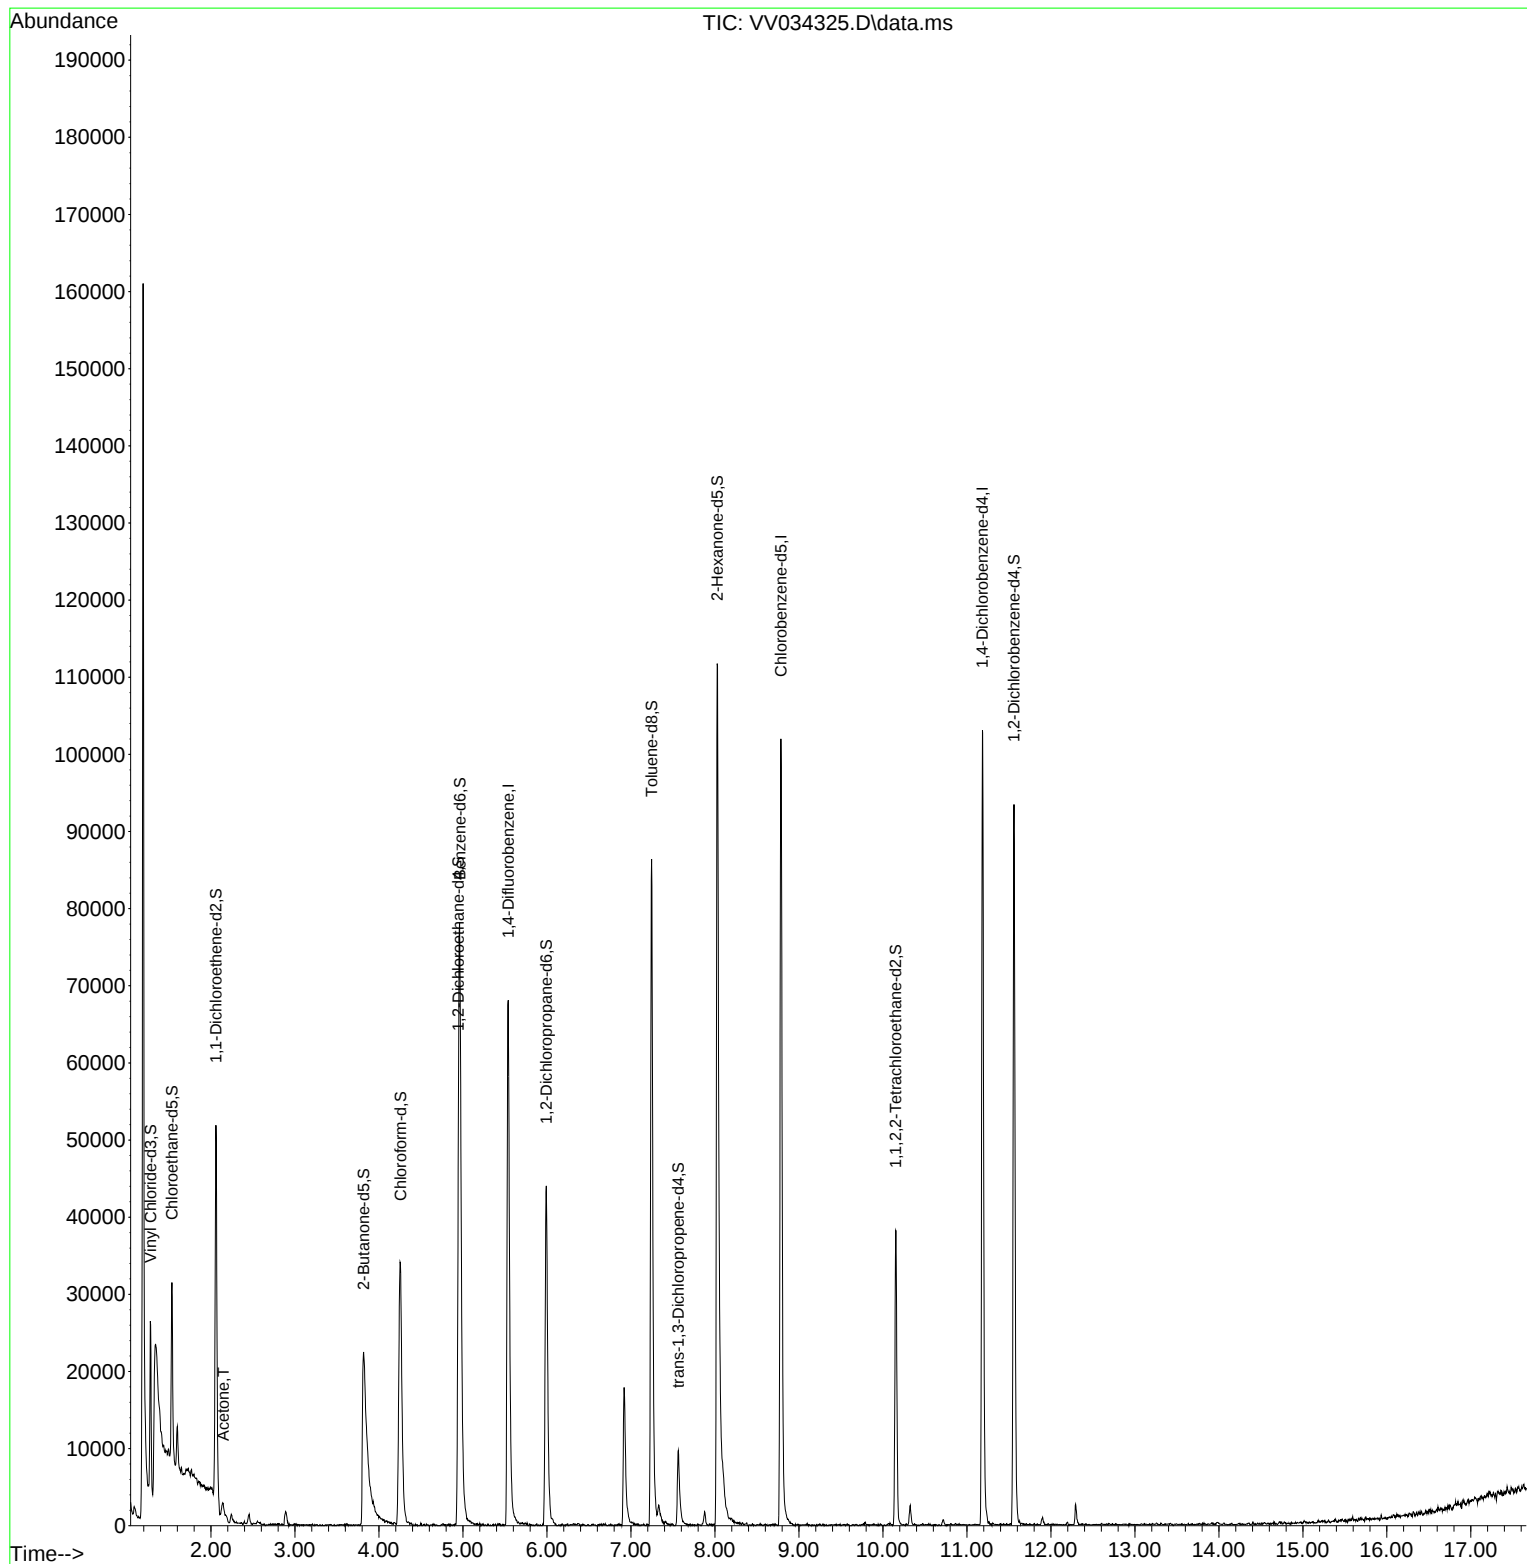

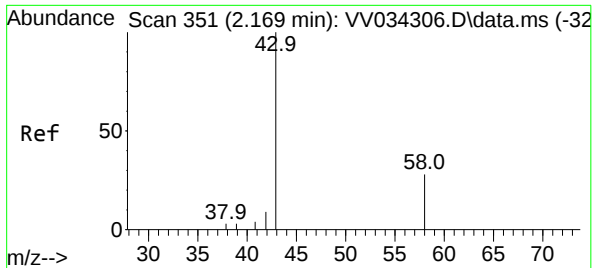

#13
 Acetone
 Concen: 7.703 ug/L
 RT: 2.146 min Scan# 34
 Delta R.T. -0.023 min
 Lab File: VV034325.D
 Acq: 21 Feb 2024 17:33

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH3

Tgt Ion: 43 Resp: 4590
 Ion Ratio Lower Upper
 43 100
 58 12.2 0.0 13.8

