


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022124\
Data File : VV034305.D
Acq On : 21 Feb 2024 08:37
Operator : SY/MD
Sample : BFB257
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB257

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Feb 22 00:18:57 2024

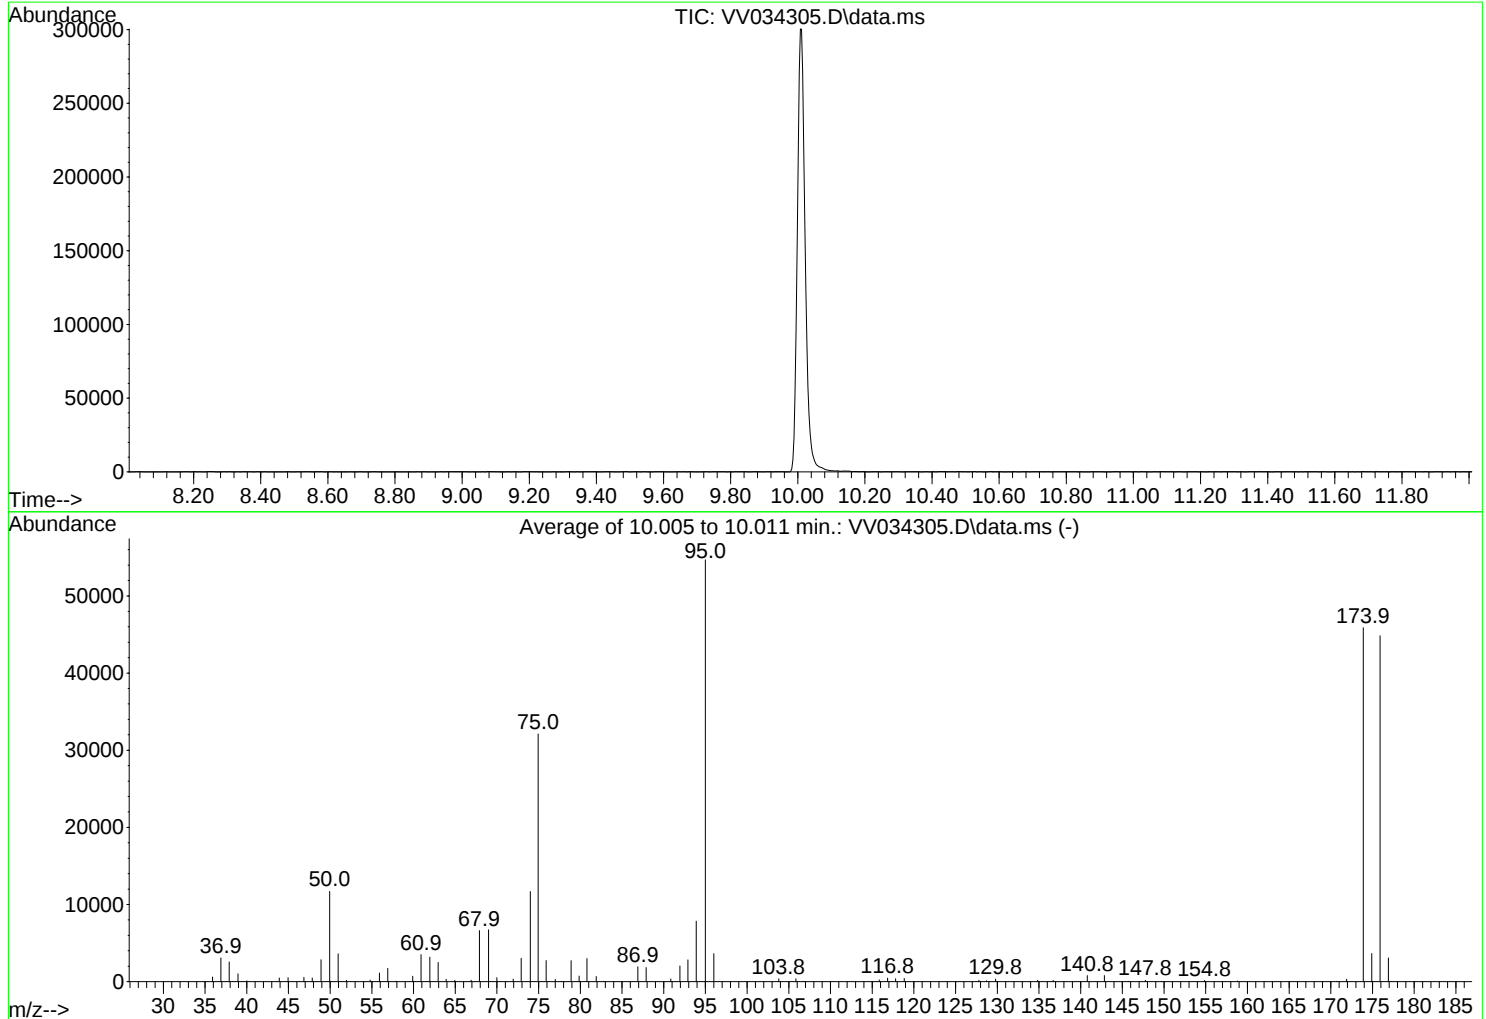

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	11706	PASS
75	95	30	80	58.7	32109	PASS
95	95	100	100	100.0	54683	PASS
96	95	5	9	6.7	3641	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.9	45893	PASS
175	174	5	9	8.0	3654	PASS
176	174	95	105	97.7	44848	PASS
177	176	5	10	6.8	3065	PASS

m/z	Abundance
74.80	119.0
94.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

m/z	Abundance
35.90	586.0
36.90	2870.0
37.90	2475.0
39.00	965.0
40.00	102.0
43.90	443.0
44.90	478.0
46.80	563.0
47.90	480.0
48.90	2781.0
49.90	11334.0
51.00	3397.0
52.00	145.0
54.80	209.0
55.90	1092.0
56.90	1625.0
59.90	656.0
60.90	3296.0
61.90	3050.0
62.90	2386.0
63.90	311.0
64.90	164.0
66.90	149.0
67.90	6173.0
69.00	6331.0
70.00	475.0
72.00	318.0
72.90	2799.0
74.00	11309.0
75.00	30376.0
75.90	2644.0
77.00	293.0
78.90	2589.0
79.90	740.0
80.80	2892.0
81.90	642.0
82.80	109.0
86.90	1823.0
87.90	1727.0
90.80	337.0
91.90	1799.0
92.90	2489.0
93.90	7244.0
95.00	51112.0
96.00	3420.0
103.80	320.0
105.80	381.0
115.90	245.0
116.90	423.0
117.80	358.0
118.90	349.0
127.80	181.0
128.70	118.0
129.80	294.0
134.80	172.0
136.70	152.0
140.80	751.0
142.90	720.0
147.70	150.0
154.80	134.0
158.80	131.0
171.80	294.0
173.90	42008.0
174.90	3495.0
175.90	40704.0
176.90	2850.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

m/z	Abundance
35.90	621.0
36.90	3179.0
37.90	2597.0
38.90	1048.0
40.00	124.0
43.90	487.0
44.90	528.0
46.90	558.0
47.90	505.0
48.90	2928.0
50.00	12044.0
51.00	3750.0
52.00	178.0
54.80	208.0
55.90	1127.0
56.90	1759.0
57.90	104.0
59.90	717.0
60.90	3647.0
62.00	3256.0
62.90	2573.0
63.90	322.0
65.00	167.0
66.90	176.0
67.90	6865.0
69.00	6920.0
70.00	531.0
72.00	344.0
72.90	3090.0
74.00	12030.0
74.90	33240.0
75.90	2816.0
77.00	297.0
78.90	2823.0
79.90	734.0
80.80	3076.0
81.90	691.0
86.90	2018.0
87.90	1864.0
90.90	370.0
92.00	2141.0
92.90	2927.0
93.90	8143.0
95.00	56640.0
96.00	3773.0
103.80	379.0
105.80	385.0
115.90	217.0
116.80	455.0
117.80	394.0
118.80	407.0
127.80	195.0
128.70	119.0
129.80	351.0
134.90	161.0
136.70	163.0
140.80	801.0
142.80	797.0
147.70	178.0
154.80	144.0
158.80	128.0
171.90	322.0
173.90	47480.0
174.90	3777.0
175.90	46432.0
176.90	3157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

m/z	Abundance
35.90	578.0
36.90	3150.0
37.90	2564.0
38.90	1036.0
40.00	115.0
43.90	496.0
45.00	523.0
46.90	537.0
47.80	478.0
48.90	2806.0
50.00	11739.0
50.90	3666.0
51.90	187.0
54.80	176.0
55.90	1122.0
56.90	1791.0
57.90	108.0
59.90	733.0
60.90	3562.0
62.00	3190.0
63.00	2493.0
63.90	315.0
65.00	143.0
66.90	211.0
67.90	6838.0
69.00	6918.0
70.00	531.0
71.90	342.0
72.90	3187.0
74.00	11727.0
74.90	32712.0
75.90	2761.0
77.00	295.0
77.70	121.0
78.90	2759.0
79.80	727.0
80.80	2973.0
81.90	674.0
86.90	1968.0
87.90	1861.0
90.90	348.0
92.00	2140.0
92.90	3053.0
93.90	8118.0
95.00	56296.0
96.00	3729.0
103.80	406.0
105.90	334.0
106.80	111.0
115.80	208.0
116.80	505.0
117.80	365.0
118.80	479.0
127.80	201.0
128.70	110.0
129.80	337.0
134.90	144.0
136.70	166.0
140.80	817.0
142.80	842.0
145.70	104.0
147.80	182.0
149.70	110.0
154.90	147.0
170.70	102.0
172.00	333.0
173.90	48192.0
174.90	3689.0
175.90	47408.0
176.90	3187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257