
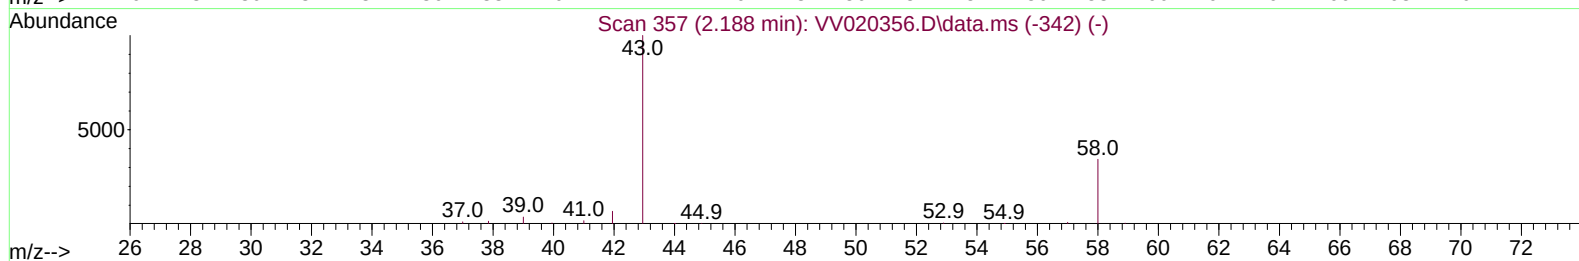
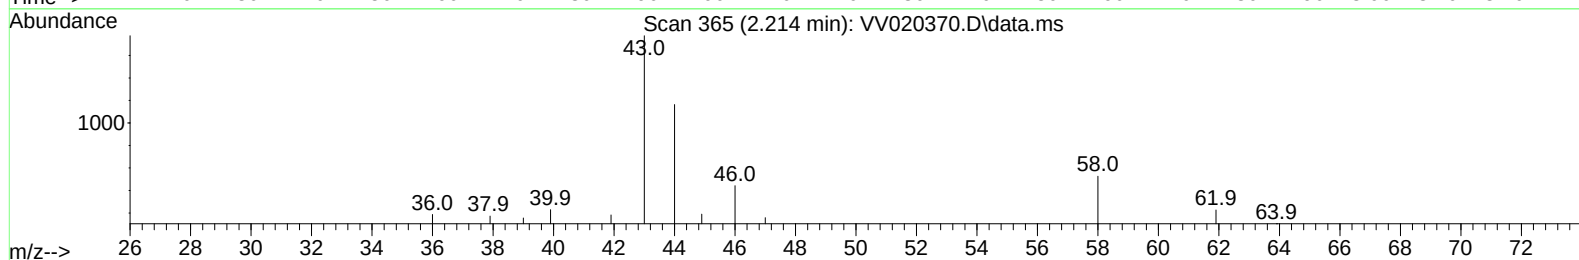


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022221\
 Data File : VV020370.D
 Acq On : 22 Feb 2021 19:02
 Operator : SY/MD
 Sample : M1468-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 02:29:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Feb 23 02:26:51 2021
 Response via : Initial Calibration

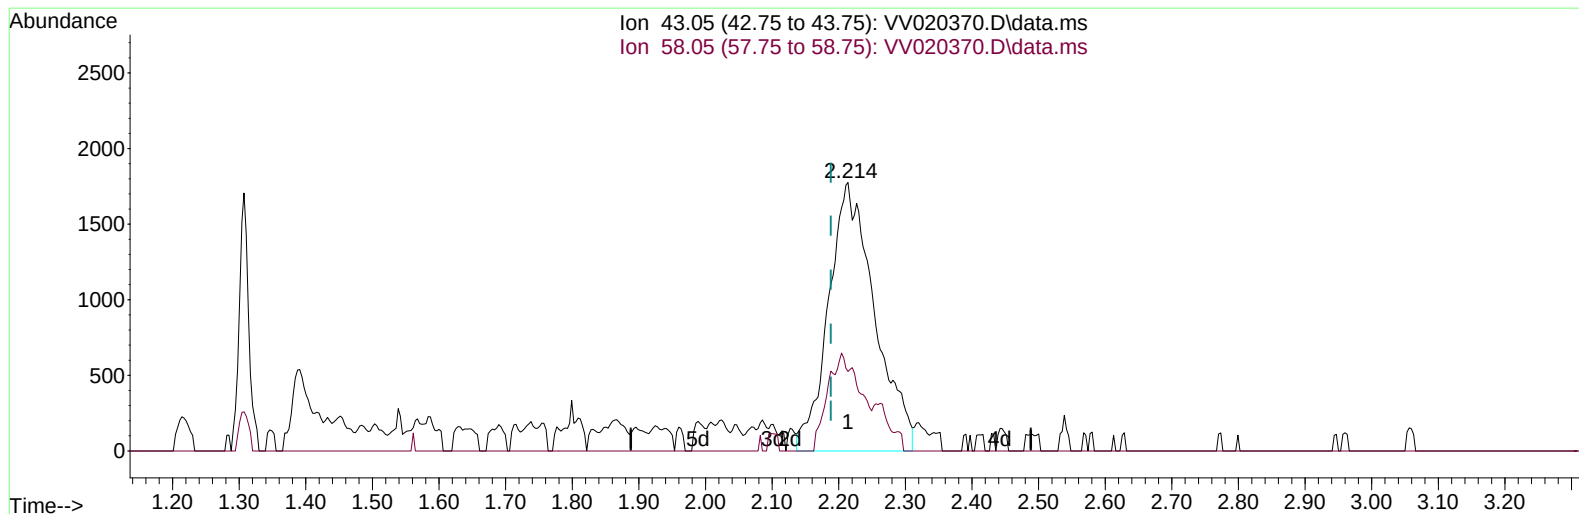

TIC: VV020370.D\data.ms

(13) Acetone (T)




2.214min (+ 0.026) 2.57 ug/L m

response 8518

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	9.30	15.50
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022221\
 Data File : VV020370.D
 Acq On : 22 Feb 2021 19:02
 Operator : SY/MD
 Sample : M1468-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 02:29:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Feb 23 02:26:51 2021
 Response via : Initial Calibration

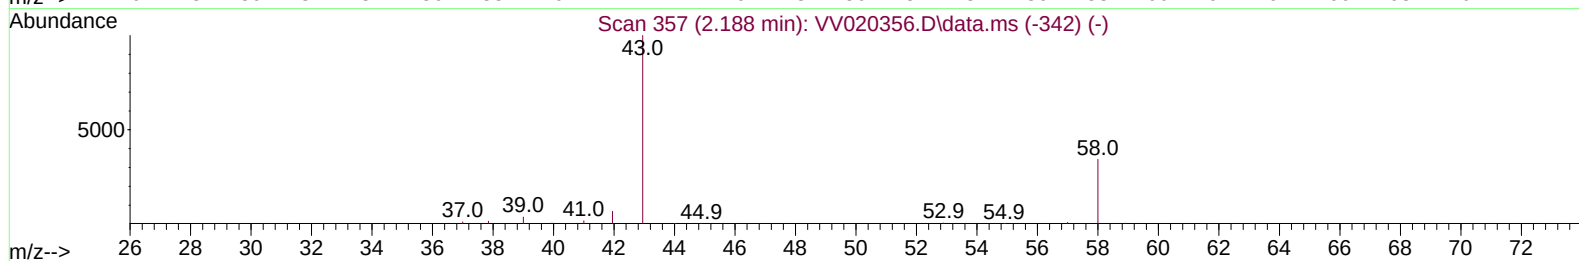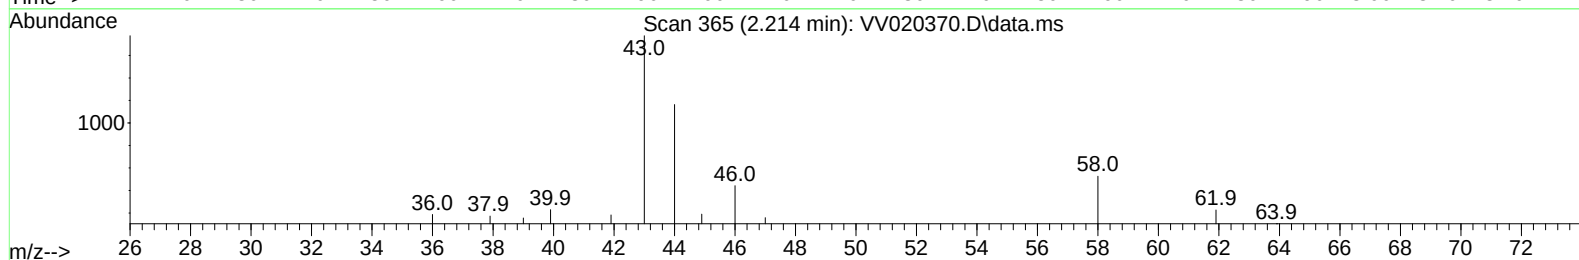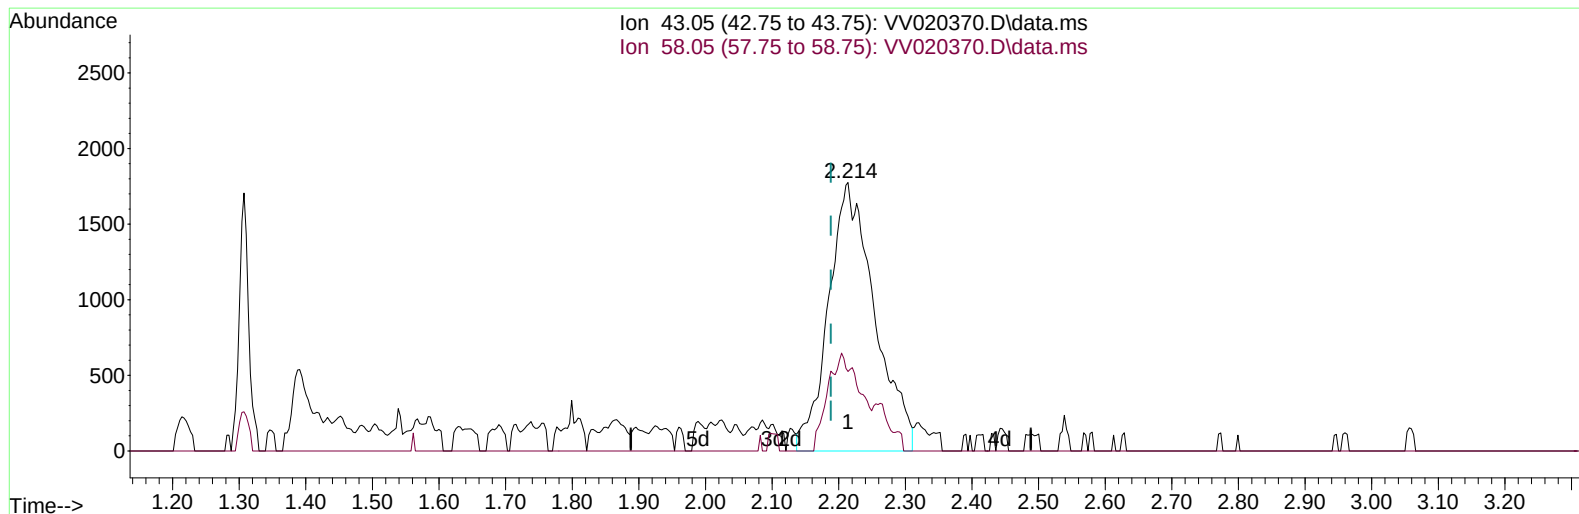

TIC: VV020370.D\data.ms

(13) Acetone (T)

2.214min (+ 0.026) 2.57 ug/L m

response 8518

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	9.30	15.50
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022221\
 Data File : VV020370.D
 Acq On : 22 Feb 2021 19:02
 Operator : SY/MD
 Sample : M1468-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 02:29:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Feb 23 02:26:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	299936	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	288057	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.255	152	135198	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	115342	5.46	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.20%
7) Chloroethane-d5	1.568	69	88188	5.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.20%
11) 1,1-Dichloroethene-d2	2.108	63	152058	3.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.00%
20) 2-Butanone-d5	3.908	46	184341	50.39	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.78%
24) Chloroform-d	4.352	84	183852	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
26) 1,2-Dichloroethane-d4	5.037	65	92395	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
32) Benzene-d6	5.053	84	373133	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.40%
36) 1,2-Dichloropropane-d6	6.076	67	110290	5.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.20%
41) Toluene-d8	7.320	98	342917	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
45) trans-1,3-Dichloroprop...	7.629	79	36704	4.50	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.00%
48) 2-Hexanone-d5	8.095	63	122314	42.74	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.48%
59) 1,1,2,2-Tetrachloroeth...	10.223	84	67168	4.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.40%
65) 1,2-Dichlorobenzene-d4	11.632	152	128960	5.38	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.60%
Target Compounds						
					Qvalue	
13) Acetone	2.214	43	8518m	2.57	ug/L	
14) Carbon disulfide	2.298	76	9828	0.12	ug/L	96
22) cis-1,2-Dichloroethene	3.918	96	154794	5.56	ug/L	95
50) 2-Hexanone	8.146	43	12993	1.50	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022221\
Data File : VV020370.D
Acq On : 22 Feb 2021 19:02
Operator : SY/MD
Sample : M1468-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 02:29:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Feb 23 02:26:51 2021
Response via : Initial Calibration

