

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022221\
 Data File : VV020372.D
 Acq On : 22 Feb 2021 19:49
 Operator : SY/MD
 Sample : M1468-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Feb 23 02:29:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Feb 23 02:26:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	327302	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	316645	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.255	152	151150	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	96495	4.19	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.80%
7) Chloroethane-d5	1.568	69	79756	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.00%
11) 1,1-Dichloroethene-d2	2.108	63	130243	2.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.00%#
20) 2-Butanone-d5	3.899	46	168374	42.17	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.34%
24) Chloroform-d	4.352	84	167634	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.40%
26) 1,2-Dichloroethane-d4	5.037	65	88510	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.40%
32) Benzene-d6	5.053	84	341716	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.20%
36) 1,2-Dichloropropane-d6	6.075	67	102089	4.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.00%
41) Toluene-d8	7.320	98	304969	3.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.60%
45) trans-1,3-Dichloroprop...	7.628	79	34373	3.83	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.60%
48) 2-Hexanone-d5	8.091	63	111101	35.31	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	70.62%
59) 1,1,2,2-Tetrachloroeth...	10.223	84	61787	3.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	74.00%
65) 1,2-Dichlorobenzene-d4	11.631	152	123100	4.59	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.80%
Target Compounds					Qvalue	
50) 2-Hexanone	8.149	43	14997	1.58	ug/L #	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022221\
Data File : VV020372.D
Acq On : 22 Feb 2021 19:49
Operator : SY/MD
Sample : M1468-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Feb 23 02:29:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Feb 23 02:26:51 2021
Response via : Initial Calibration

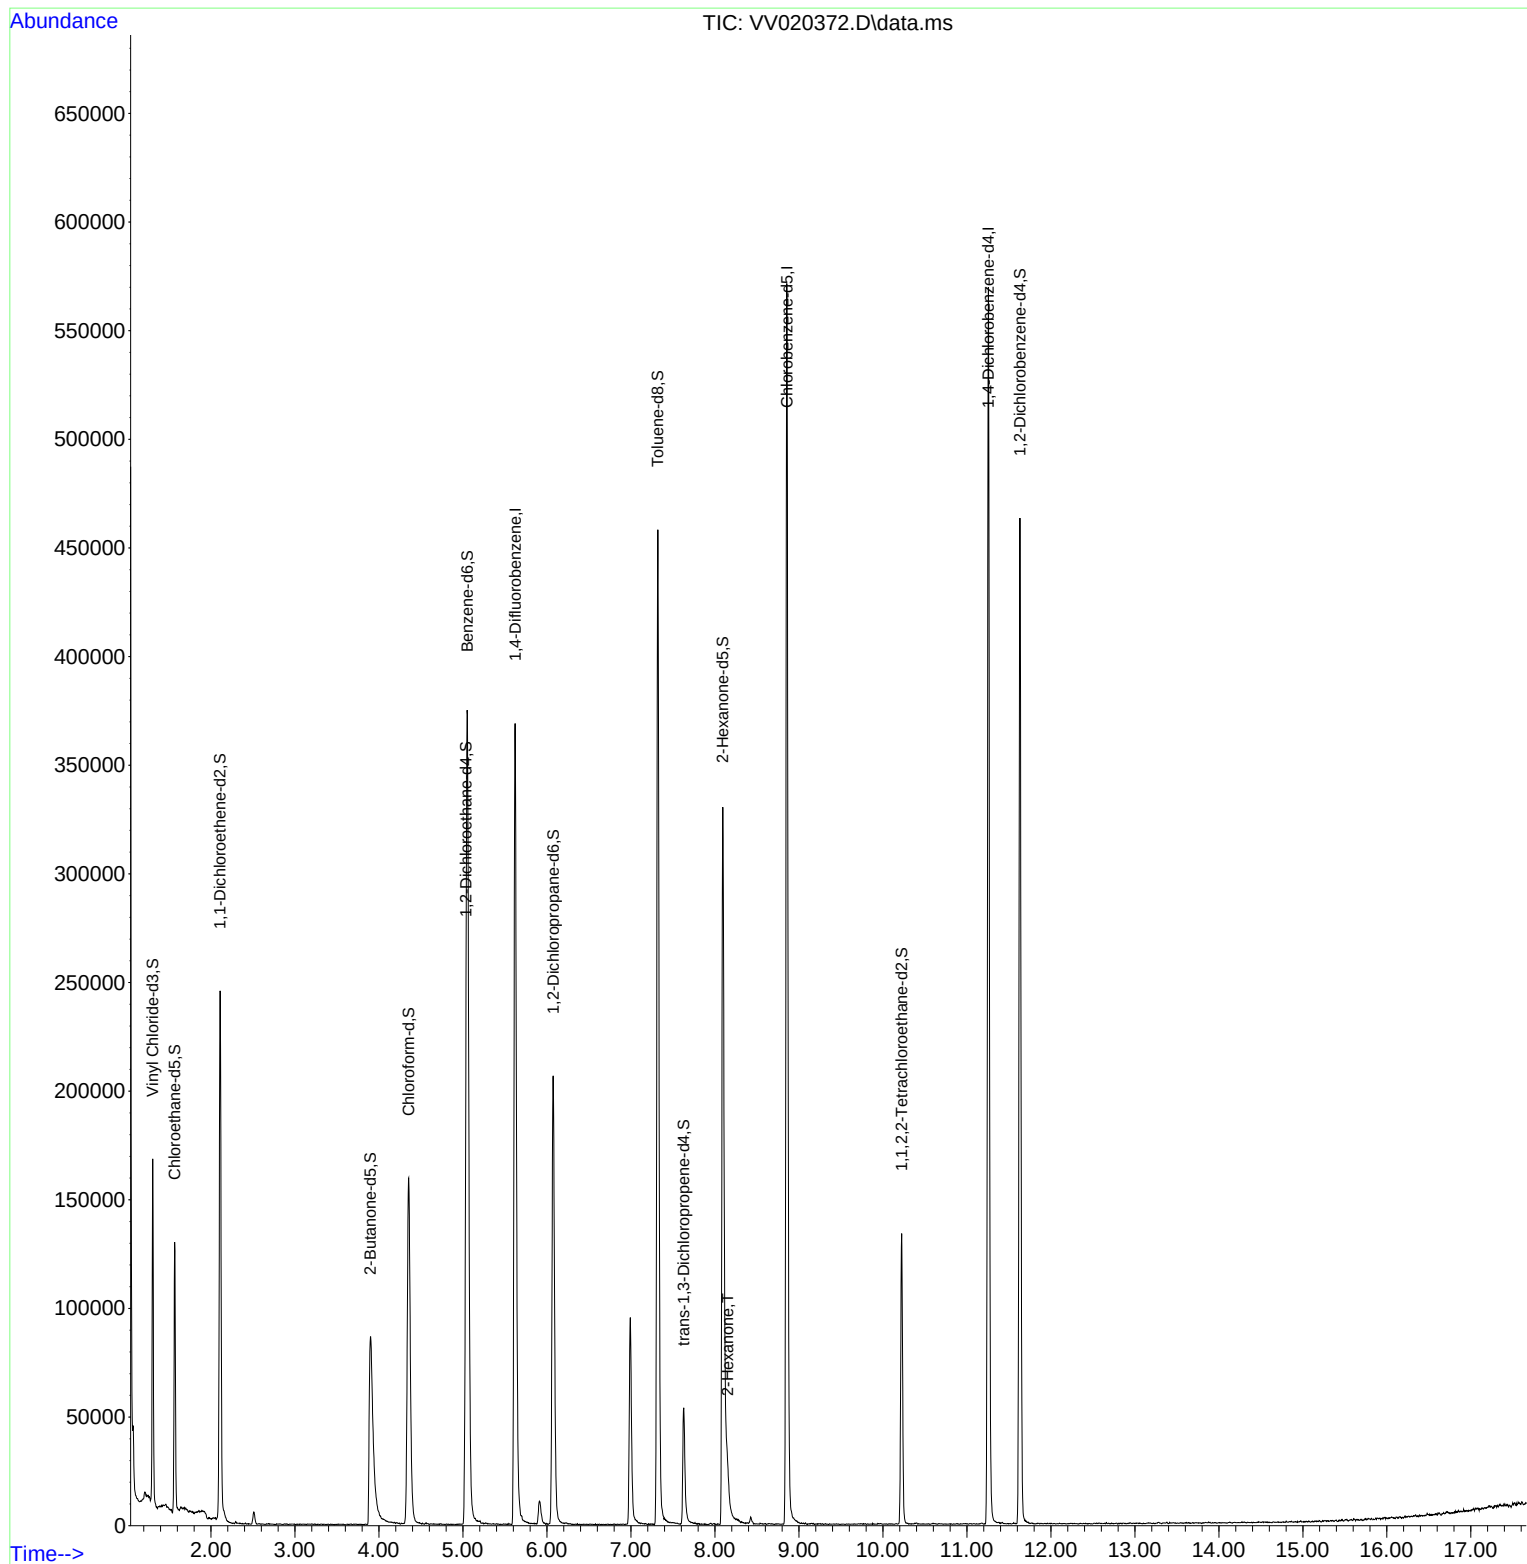

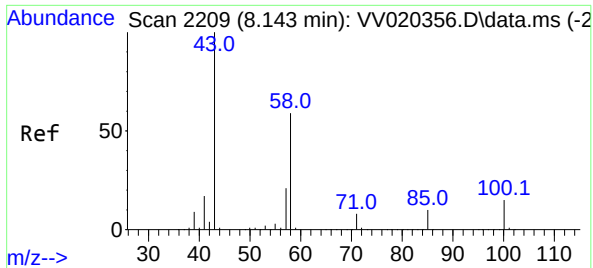

#50
2-Hexanone
Concen: 1.58 ug/L
RT: 8.149 min Scan# 2211
Delta R.T. 0.006 min
Lab File: VV020372.D
Acq: 22 Feb 2021 19:49

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Tgt Ion: 43 Resp: 14997

Ion	Ratio	Lower	Upper
43	100		
58	41.8	41.6	62.4
57	12.1	15.4	23.0#
100	5.6	11.2	16.8#

