
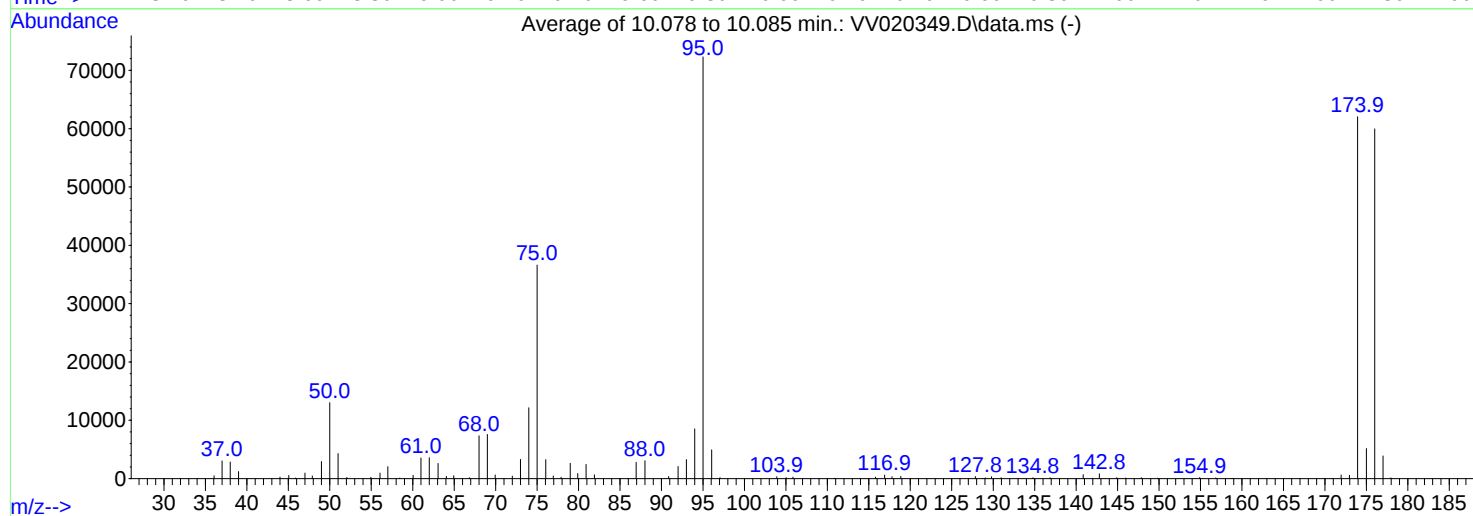


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022221\
Data File : VV020349.D
Acq On : 22 Feb 2021 09:10
Operator : SY/MD
Sample : BFB31
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB31

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Feb 23 02:26:51 2021

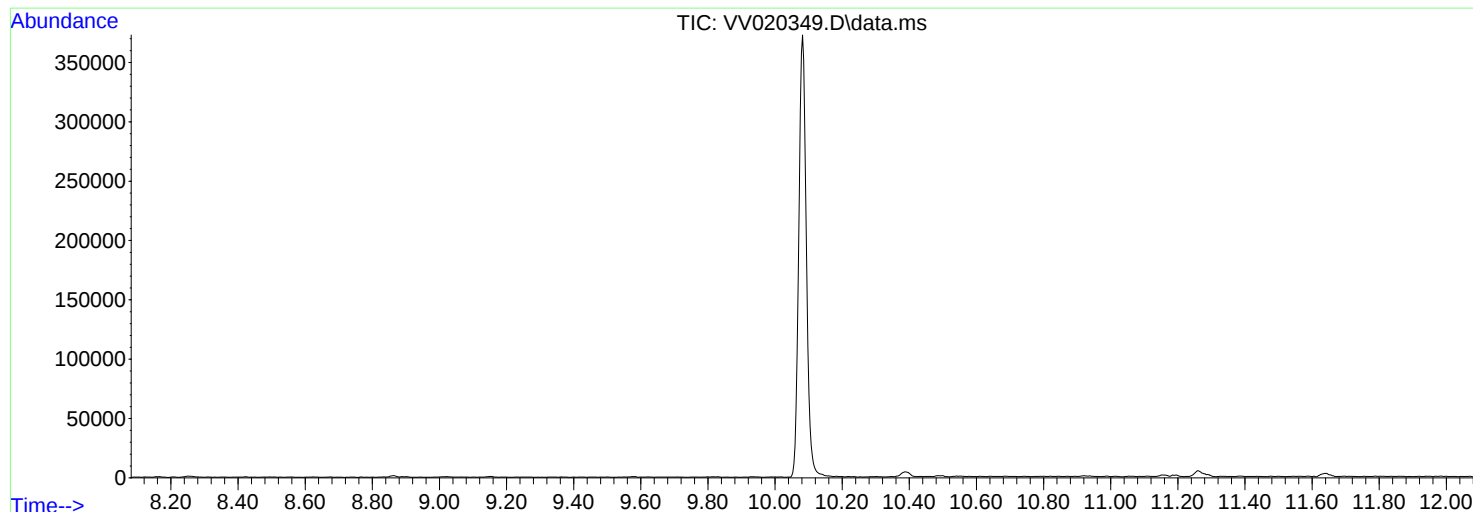

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	13037	PASS
75	95	30	80	50.6	36627	PASS
95	95	100	100	100.0	72317	PASS
96	95	5	9	6.8	4953	PASS
173	174	0.00	2	0.9	586	PASS
174	95	50	120	85.8	62067	PASS
175	174	5	9	8.3	5162	PASS
176	174	95	101	96.6	59981	PASS
177	176	5	9	6.5	3896	PASS

m/z	Abundance
36.00	553.0
37.00	3123.0
38.00	2896.0
39.00	1204.0
40.00	252.0
44.00	811.0
45.10	559.0
45.80	134.0
47.00	1034.0
47.90	563.0
49.00	2957.0
50.00	13041.0
51.00	4518.0
52.00	238.0
54.90	209.0
56.00	987.0
57.00	2066.0
58.50	106.0
60.00	602.0
61.00	3606.0
62.00	3467.0
63.00	2601.0
64.00	371.0
65.00	512.0
67.00	178.0
68.00	7465.0
69.00	7545.0
70.00	632.0
72.00	401.0
73.00	3124.0
74.00	12175.0
75.00	36712.0
76.10	3267.0
76.90	436.0
77.90	244.0
79.00	2648.0
79.90	881.0
80.90	2492.0
81.90	547.0
86.90	2857.0
88.00	2810.0
90.90	309.0
92.00	2156.0
93.00	3282.0
94.00	8770.0
95.00	72336.0
96.00	4993.0
97.00	164.0
103.90	352.0
105.00	156.0
105.80	219.0
110.80	107.0
115.80	250.0
116.90	561.0
117.80	324.0
118.90	358.0
127.80	387.0
129.00	130.0
129.80	316.0
130.90	142.0
134.80	158.0
136.80	127.0
140.90	775.0
141.90	113.0
142.80	739.0
144.90	147.0
146.00	109.0
147.90	135.0
149.90	122.0
154.90	173.0
156.90	154.0
171.90	631.0
172.90	577.0
173.90	60512.0
175.00	5035.0
176.00	58120.0
177.00	3889.0
178.00	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
36.00	504.0
37.00	3166.0
38.00	2977.0
39.00	1244.0
39.90	238.0
44.00	748.0
45.10	564.0
45.90	124.0
47.00	1023.0
47.90	468.0
49.00	3027.0
50.00	13497.0
51.00	4475.0
52.00	241.0
55.00	252.0
56.00	967.0
57.00	2154.0
58.50	121.0
60.10	588.0
61.00	3689.0
62.00	3752.0
63.10	2691.0
64.10	416.0
65.00	494.0
66.80	168.0
68.00	7669.0
69.00	7861.0
70.00	652.0
72.00	460.0
73.00	3433.0
74.00	12596.0
75.00	37824.0
76.10	3371.0
76.90	494.0
77.90	228.0
79.00	2750.0
79.90	900.0
80.90	2553.0
81.90	678.0
87.00	2822.0
88.00	3223.0
90.90	377.0
92.00	2135.0
93.00	3337.0
94.00	8855.0
95.00	74784.0
96.00	5175.0
97.00	156.0
103.90	326.0
105.00	173.0
105.90	281.0
110.90	107.0
115.80	276.0
116.90	629.0
117.80	355.0
118.80	373.0
127.80	346.0
129.10	143.0
129.80	339.0
131.00	165.0
134.80	176.0
136.80	163.0
140.80	699.0
142.00	103.0
142.80	876.0
144.90	175.0
146.00	123.0
147.90	171.0
149.80	115.0
154.90	185.0
156.90	140.0
158.80	107.0
172.00	620.0
172.90	617.0
173.90	64040.0
175.00	5394.0
176.00	61816.0
177.00	4045.0
177.90	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
36.10	422.0
37.00	2825.0
38.00	2713.0
39.00	1181.0
39.90	229.0
44.00	700.0
45.00	509.0
45.90	117.0
47.00	813.0
47.90	350.0
49.00	2829.0
50.00	12572.0
51.00	3951.0
52.10	191.0
54.90	299.0
56.10	941.0
57.00	1990.0
58.40	108.0
60.10	536.0
61.00	3368.0
62.00	3594.0
63.10	2560.0
64.10	395.0
64.90	459.0
66.80	147.0
68.00	6949.0
69.00	7279.0
69.90	583.0
72.00	448.0
73.00	3354.0
74.00	11725.0
75.00	35344.0
76.00	3121.0
77.00	506.0
77.90	262.0
79.00	2483.0
79.90	851.0
80.90	2267.0
81.90	727.0
85.90	122.0
87.00	2710.0
88.00	3173.0
90.80	374.0
92.00	1985.0
93.00	3207.0
94.00	7945.0
95.00	69832.0
96.10	4692.0
97.10	150.0
103.90	347.0
105.10	139.0
105.90	319.0
115.80	285.0
116.90	618.0
117.80	304.0
118.80	406.0
127.90	303.0
128.70	126.0
129.10	147.0
129.80	327.0
131.00	162.0
134.80	156.0
136.90	171.0
140.80	614.0
142.80	865.0
144.90	201.0
145.90	142.0
147.80	180.0
154.90	214.0
156.80	114.0
158.80	106.0
170.80	102.0
172.00	622.0
173.00	563.0
174.00	61648.0
175.00	5058.0
176.00	60008.0
177.00	3755.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
39.80	275.0
44.00	463.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31