

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022223\
 Data File : VV030078.D
 Acq On : 22 Feb 2023 13:02
 Operator : SY/MD
 Sample : VV0222MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK318

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	52	56	64	rBV2	5215	6245	0.44%	0.056%
2	1.281	68	75	94	rVB	226996	245392	17.20%	2.189%
3	1.535	147	154	171	rVB	188937	224056	15.70%	1.999%
4	2.066	308	319	338	rBV	385805	557233	39.05%	4.971%
5	2.346	403	406	408	rBV	287	157	0.01%	0.001%
6	2.375	412	415	418	rBV2	228	149	0.01%	0.001%
7	2.455	432	440	449	rVB2	3309	5294	0.37%	0.047%
8	2.519	455	460	462	rBV2	247	245	0.02%	0.002%
9	2.696	512	515	517	rVV2	293	195	0.01%	0.002%
10	2.940	584	591	595	rBV	252	280	0.02%	0.002%
11	2.963	595	598	604	rVB2	225	253	0.02%	0.002%
12	3.027	613	618	622	rBV2	205	197	0.01%	0.002%
13	3.143	651	654	658	rBV2	189	153	0.01%	0.001%
14	3.336	709	714	717	rVB2	181	168	0.01%	0.001%
15	3.355	717	720	726	rVB	276	265	0.02%	0.002%
16	3.580	787	790	795	rVB2	376	239	0.02%	0.002%
17	3.606	795	798	805	rBV2	192	230	0.02%	0.002%
18	3.635	805	807	812	rVB	225	179	0.01%	0.002%
19	3.799	847	858	895	rBV	94947	274246	19.22%	2.447%
20	4.259	984	1001	1025	rBV	221714	563086	39.46%	5.024%
21	4.513	1078	1080	1085	rVB3	269	149	0.01%	0.001%
22	4.567	1095	1097	1099	rBV	275	187	0.01%	0.002%
23	4.966	1202	1221	1249	rBV2	542339	1426990	100.00%	12.731%
24	5.400	1352	1356	1358	rVV2	231	176	0.01%	0.002%
25	5.461	1369	1375	1379	rBV2	271	280	0.02%	0.002%
26	5.542	1384	1400	1429	rBV	403178	820757	57.52%	7.323%
27	5.831	1482	1490	1493	rBV5	1515	2050	0.14%	0.018%
28	5.892	1501	1509	1515	rBV3	292	443	0.03%	0.004%
29	5.998	1526	1542	1564	rBV	305758	632836	44.35%	5.646%
30	6.239	1614	1617	1620	rBV2	197	145	0.01%	0.001%
31	6.307	1635	1638	1644	rBV2	164	151	0.01%	0.001%
32	6.394	1659	1665	1669	rBV2	223	177	0.01%	0.002%
33	6.561	1709	1717	1718	rBV5	992	1171	0.08%	0.010%
34	6.725	1765	1768	1770	rBV	189	147	0.01%	0.001%
35	6.921	1816	1829	1857	rBV	171841	319514	22.39%	2.851%
36	7.079	1875	1878	1879	rBV	618	284	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022223\
 Data File : VV030078.D
 Acq On : 22 Feb 2023 13:02
 Operator : SY/MD
 Sample : VV0222MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK318

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
 Title : VOC Analysis

37	7.120	1889	1891	1895	rVB4	400	221	0.02%	0.002%
38	7.252	1918	1932	1969	rBV	678734	1195205	83.76%	10.663%
39	7.484	2002	2004	2011	rVB4	415	496	0.03%	0.004%
40	7.558	2016	2027	2054	rBV	119536	212456	14.89%	1.895%
41	7.918	2135	2139	2142	rVB2	315	259	0.02%	0.002%
42	7.953	2147	2150	2154	rBV3	255	198	0.01%	0.002%
43	8.030	2162	2174	2208	rBV	343187	605187	42.41%	5.399%
44	8.278	2245	2251	2253	rBV3	243	232	0.02%	0.002%
45	8.371	2270	2280	2288	rBV3	3627	6311	0.44%	0.056%
46	8.792	2398	2411	2439	rBV	605907	1008217	70.65%	8.995%
47	8.956	2460	2462	2463	rBV2	340	149	0.01%	0.001%
48	9.078	2497	2500	2503	rBV2	332	240	0.02%	0.002%
49	9.123	2509	2514	2518	rBV2	261	242	0.02%	0.002%
50	9.226	2544	2546	2549	rVB2	224	149	0.01%	0.001%
51	9.487	2621	2627	2630	rBV3	302	341	0.02%	0.003%
52	9.506	2630	2633	2634	rBV2	513	253	0.02%	0.002%
53	9.583	2652	2657	2662	rBV2	169	218	0.02%	0.002%
54	9.628	2668	2671	2677	rVB	218	170	0.01%	0.002%
55	9.680	2683	2687	2690	rBV2	191	183	0.01%	0.002%
56	9.757	2707	2711	2715	rBV2	160	176	0.01%	0.002%
57	9.805	2722	2726	2732	rBV2	156	179	0.01%	0.002%
58	9.876	2743	2748	2757	rBV2	441	667	0.05%	0.006%
59	10.037	2794	2798	2803	rVB2	198	181	0.01%	0.002%
60	10.069	2803	2808	2811	rBV2	165	184	0.01%	0.002%
61	10.162	2824	2837	2859	rBV	457429	726404	50.90%	6.481%
62	10.294	2875	2878	2884	rBV2	334	310	0.02%	0.003%
63	10.493	2934	2940	2945	rBV4	631	605	0.04%	0.005%
64	10.529	2945	2951	2954	rBV2	161	197	0.01%	0.002%
65	10.725	3007	3012	3016	rBV2	189	229	0.02%	0.002%
66	10.863	3050	3055	3057	rBV3	439	377	0.03%	0.003%
67	11.008	3098	3100	3105	rVB2	217	172	0.01%	0.002%
68	11.133	3133	3139	3146	rBV2	846	1028	0.07%	0.009%
69	11.194	3146	3158	3180	rBV	762618	1168660	81.90%	10.426%
70	11.406	3219	3224	3229	rVB3	327	413	0.03%	0.004%
71	11.439	3230	3234	3236	rBV2	183	159	0.01%	0.001%
72	11.570	3262	3275	3300	rBV	748128	1157990	81.15%	10.331%
73	11.773	3334	3338	3342	rBV2	472	489	0.03%	0.004%
74	12.088	3431	3436	3438	rBV2	231	223	0.02%	0.002%
75	12.207	3464	3473	3477	rBV4	2169	2941	0.21%	0.026%
76	12.268	3490	3492	3496	rVB	321	151	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022223\
 Data File : VV030078.D
 Acq On : 22 Feb 2023 13:02
 Operator : SY/MD
 Sample : VV0222MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK318

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
 Title : VOC Analysis

77	12.438	3541	3545	3548	rBV2	398	313	0.02%	0.003%
78	12.467	3548	3554	3557	rVV	341	348	0.02%	0.003%
79	12.593	3585	3593	3599	rBV5	2114	2939	0.21%	0.026%
80	12.657	3610	3613	3615	rBV	313	203	0.01%	0.002%
81	12.747	3638	3641	3645	rVB3	318	251	0.02%	0.002%
82	12.914	3690	3693	3698	rVB2	358	266	0.02%	0.002%
83	12.940	3698	3701	3704	rBV3	293	264	0.02%	0.002%
84	13.014	3717	3724	3726	rBV2	294	313	0.02%	0.003%
85	13.046	3731	3734	3738	rVV2	453	386	0.03%	0.003%
86	13.088	3745	3747	3752	rVB2	384	301	0.02%	0.003%
87	13.159	3765	3769	3774	rBV3	480	556	0.04%	0.005%
88	13.210	3778	3785	3793	rVV3	2891	4124	0.29%	0.037%
89	13.246	3793	3796	3800	rVV2	590	469	0.03%	0.004%
90	13.274	3803	3805	3808	rVV2	348	149	0.01%	0.001%
91	13.361	3828	3832	3834	rBV	185	152	0.01%	0.001%
92	13.384	3836	3839	3843	rVV3	274	243	0.02%	0.002%
93	13.455	3853	3861	3876	rVB4	4793	7756	0.54%	0.069%
94	13.692	3927	3935	3942	rBV6	3235	4619	0.32%	0.041%
95	13.728	3942	3946	3950	rVB3	479	354	0.02%	0.003%
96	13.815	3968	3973	3976	rBV3	687	651	0.05%	0.006%
97	13.998	4020	4030	4038	rBV	3662	5725	0.40%	0.051%
98	14.069	4049	4052	4059	rVB2	595	696	0.05%	0.006%
99	14.098	4059	4061	4064	rBV	336	269	0.02%	0.002%
100	15.036	4349	4353	4357	rBV5	925	1083	0.08%	0.010%




Sum of corrected areas: 11208611

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022223\
Data File : VV030078.D
Acq On : 22 Feb 2023 13:02
Operator : SY/MD
Sample : VV0222MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

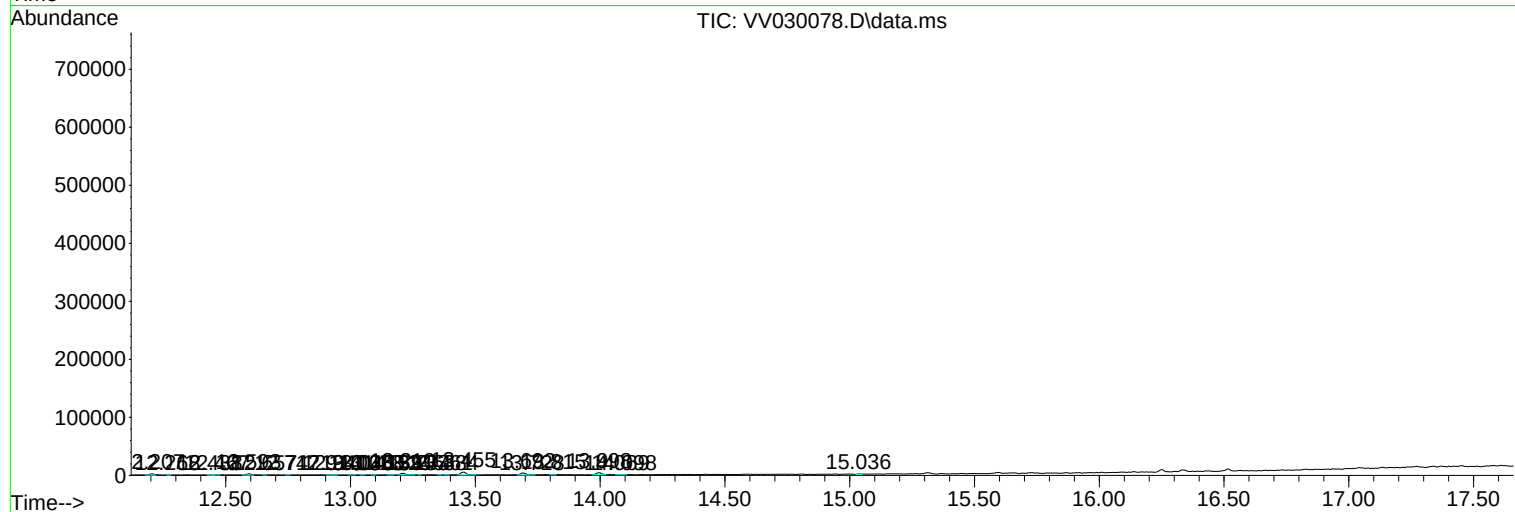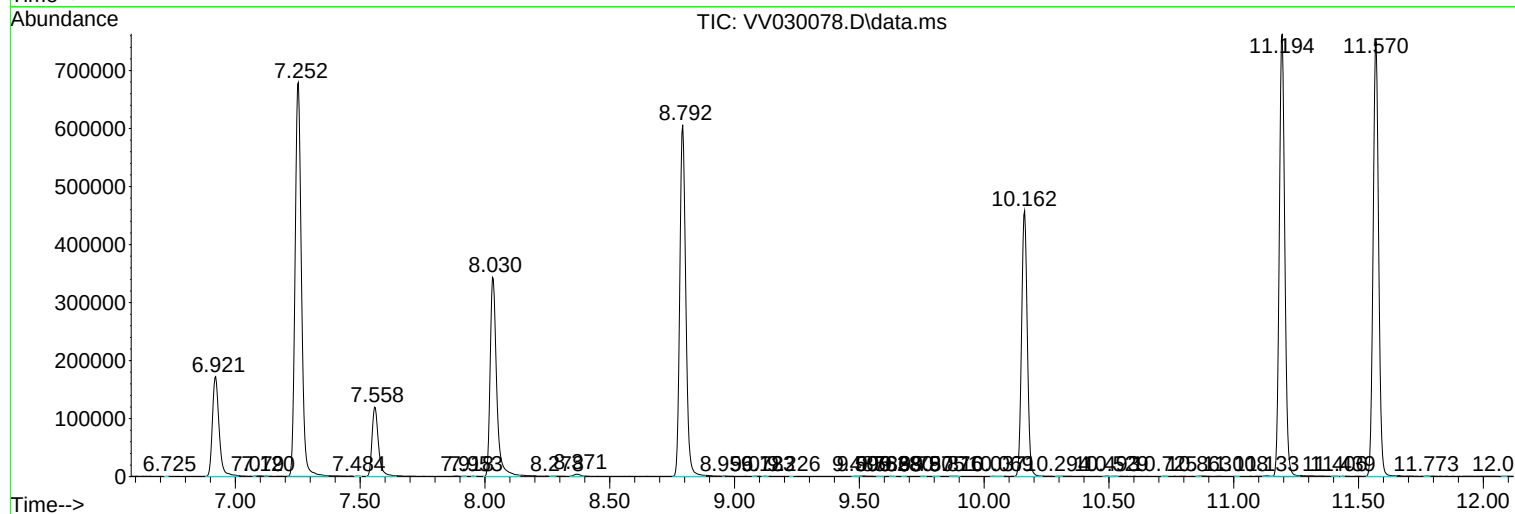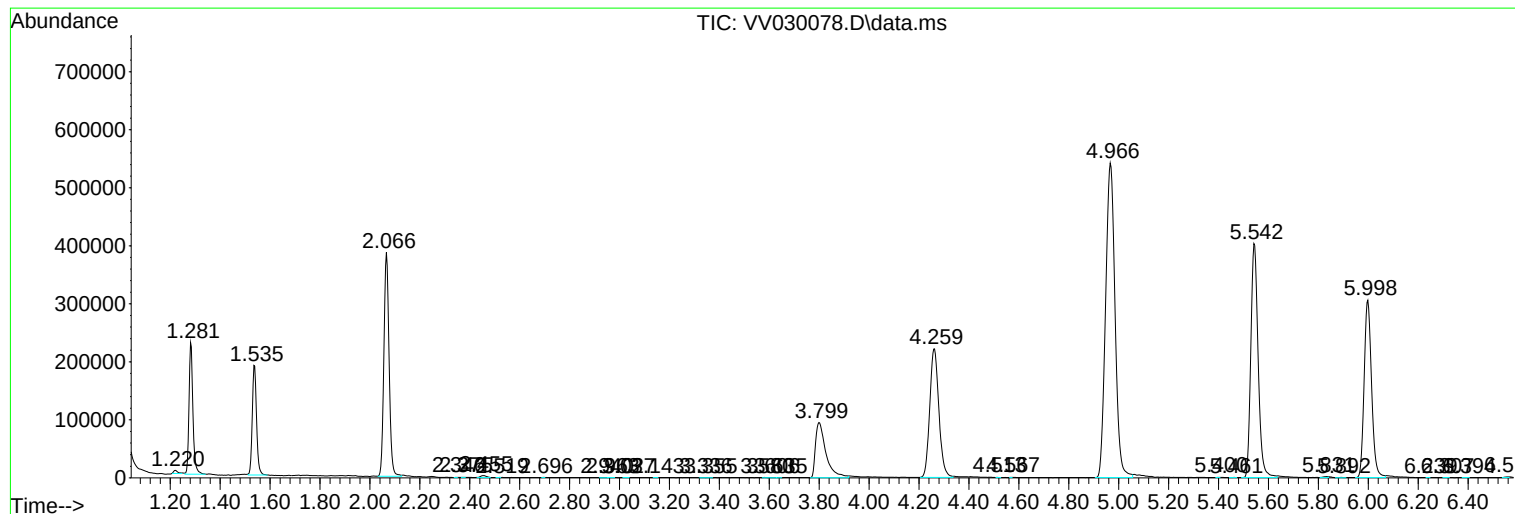

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022223\
Data File : VV030078.D
Acq On : 22 Feb 2023 13:02
Operator : SY/MD
Sample : VV0222MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022223\
Data File : VV030078.D
Acq On : 22 Feb 2023 13:02
Operator : SY/MD
Sample : VV0222MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc