
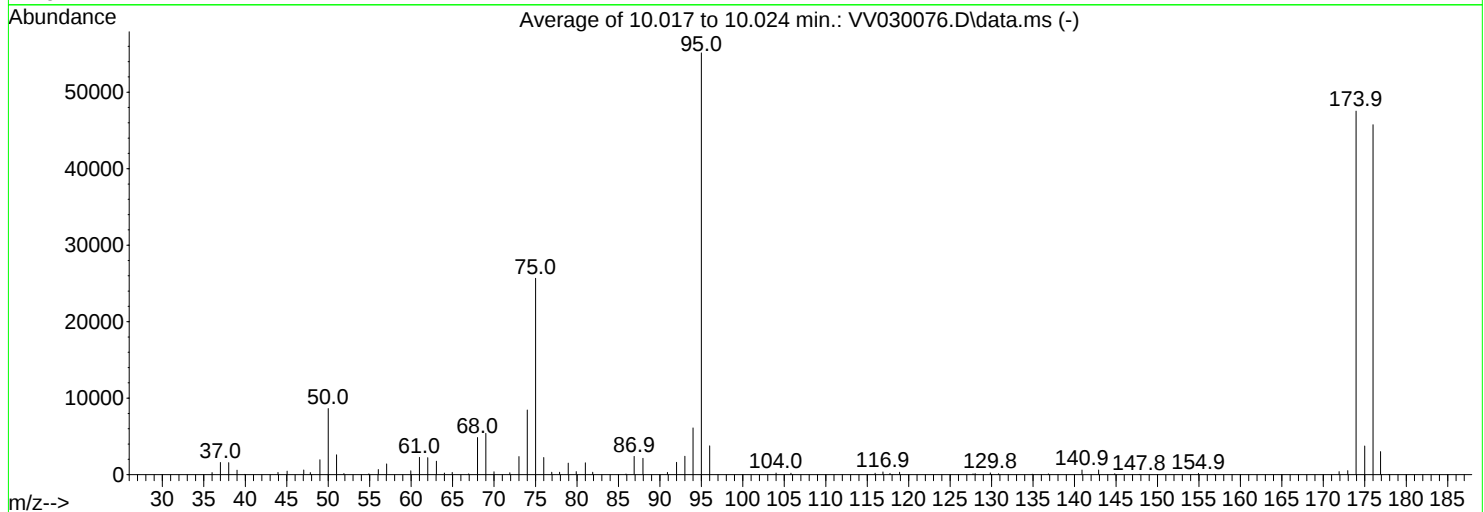


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022223\
Data File : VV030076.D
Acq On : 22 Feb 2023 10:14
Operator : SY/MD
Sample : BFB365
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB365

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
Title : VOC Analysis
Last Update : Wed Feb 22 23:16:18 2023

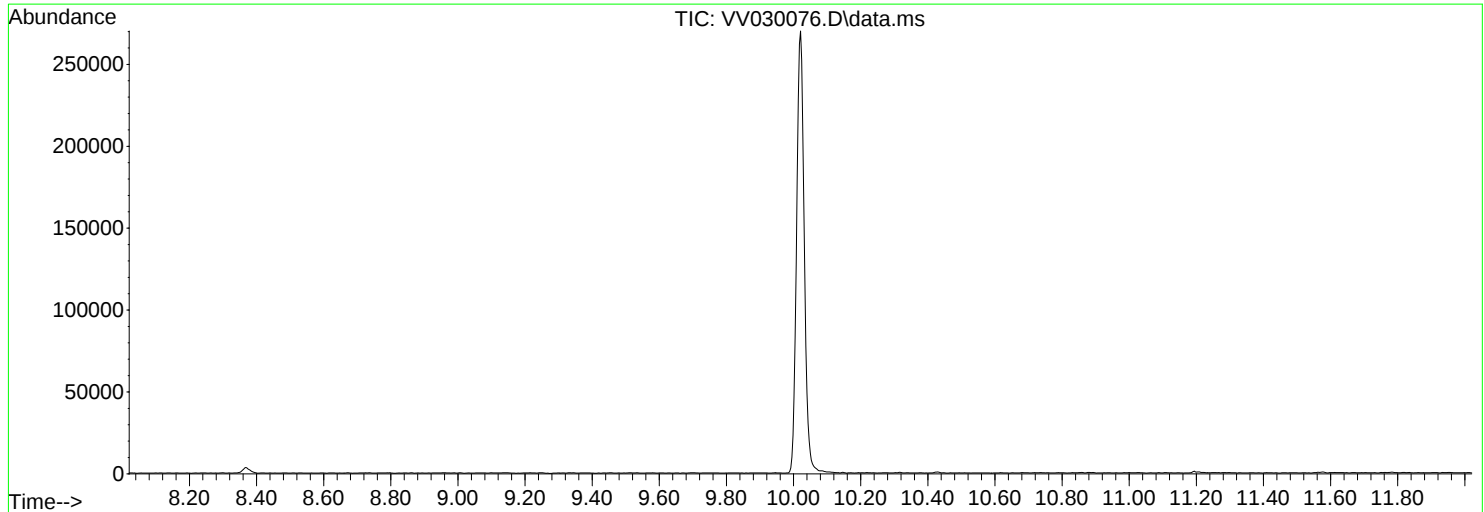

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	8640	PASS
75	95	30	80	46.5	25661	PASS
95	95	100	100	100.0	55147	PASS
96	95	5	9	6.8	3769	PASS
173	174	0.00	2	1.1	527	PASS
174	95	50	120	86.2	47523	PASS
175	174	5	9	7.9	3740	PASS
176	174	95	105	96.3	45749	PASS
177	176	5	10	6.6	3014	PASS

m/z	Abundance
39.90	138.0
44.00	433.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

m/z	Abundance
36.00	279.0
37.00	1576.0
38.00	1680.0
39.00	610.0
40.00	167.0
44.00	642.0
45.00	503.0
47.10	645.0
47.90	280.0
49.00	1881.0
50.00	8676.0
51.00	2571.0
51.90	146.0
54.90	105.0
56.10	699.0
57.00	1389.0
59.90	549.0
61.00	2402.0
62.00	2247.0
63.00	1740.0
64.00	248.0
65.00	301.0
67.00	107.0
68.00	4947.0
69.00	5365.0
70.00	326.0
71.90	310.0
73.00	2356.0
74.00	8758.0
75.00	26080.0
76.00	2319.0
77.00	328.0
77.90	309.0
79.00	1492.0
79.90	429.0
81.00	1571.0
81.90	328.0
86.90	2501.0
87.90	2198.0
90.90	273.0
92.00	1543.0
93.00	2437.0
94.00	6148.0
95.00	55776.0
96.00	3885.0
103.90	234.0
105.80	162.0
116.00	215.0
116.90	340.0
117.80	163.0
118.90	317.0
127.80	138.0
128.00	138.0
129.90	231.0
130.90	139.0
134.90	112.0
136.80	113.0
140.90	576.0
142.90	596.0
144.90	122.0
147.80	118.0
155.00	153.0
171.90	411.0
173.00	478.0
173.90	46936.0
175.00	3788.0
176.00	44712.0
176.90	3003.0
177.90	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

m/z	Abundance
36.00	284.0
37.00	1623.0
38.00	1663.0
39.00	604.0
40.00	196.0
43.90	749.0
45.00	469.0
47.00	619.0
47.90	279.0
49.00	2048.0
50.00	8962.0
51.00	2717.0
51.90	144.0
54.90	114.0
56.10	701.0
57.10	1447.0
59.90	510.0
61.00	2306.0
62.00	2256.0
63.00	1831.0
64.00	211.0
65.00	291.0
66.90	115.0
68.00	5007.0
69.00	5604.0
70.00	386.0
71.90	270.0
73.00	2443.0
74.00	8712.0
75.00	26416.0
76.00	2304.0
76.90	315.0
77.90	333.0
79.00	1575.0
79.90	408.0
81.00	1583.0
81.90	313.0
85.90	121.0
86.90	2469.0
88.00	2203.0
90.90	318.0
92.00	1648.0
93.00	2470.0
94.00	6290.0
95.00	57040.0
96.00	3890.0
104.00	203.0
105.80	185.0
115.90	185.0
116.90	356.0
117.70	172.0
118.90	316.0
127.70	159.0
128.00	155.0
129.90	232.0
130.90	136.0
134.90	106.0
136.90	118.0
140.90	627.0
142.90	619.0
144.80	124.0
154.90	155.0
171.90	407.0
172.90	553.0
173.90	49048.0
175.00	3880.0
176.00	47232.0
176.90	3151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

m/z	Abundance
36.00	287.0
37.00	1578.0
38.00	1376.0
39.00	537.0
40.00	193.0
43.90	804.0
45.10	398.0
47.00	549.0
47.80	250.0
49.00	1911.0
50.00	8282.0
51.00	2515.0
51.90	123.0
54.90	120.0
56.00	641.0
57.00	1363.0
60.00	474.0
61.00	2057.0
62.00	2146.0
63.10	1693.0
64.00	177.0
64.90	278.0
66.90	118.0
68.00	4620.0
69.00	5205.0
70.00	391.0
71.90	210.0
73.00	2282.0
74.00	7894.0
75.00	24488.0
76.00	2084.0
76.90	275.0
77.90	308.0
78.90	1472.0
79.90	366.0
81.00	1509.0
81.90	286.0
85.90	146.0
86.90	2174.0
88.00	2015.0
90.90	287.0
92.00	1624.0
93.00	2333.0
94.00	5889.0
95.00	52624.0
96.00	3533.0
104.10	190.0
105.80	207.0
115.90	162.0
116.90	344.0
117.80	162.0
118.90	290.0
128.00	171.0
129.80	215.0
130.80	119.0
136.90	111.0
140.90	631.0
142.90	578.0
144.90	129.0
154.90	167.0
156.90	104.0
171.90	393.0
172.90	551.0
174.00	46584.0
175.00	3553.0
176.00	45304.0
176.90	2887.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365