




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022224\
Data File : VV034353.D
Acq On : 22 Feb 2024 17:42
Operator : SY/MD
Sample : P1566-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAC0

Manual IntegrationsAPPROVED

Quant Time: Feb 23 01:19:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 23 01:14:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/23/2024
Supervised By :Semsettin Yesilyurt 02/23/2024

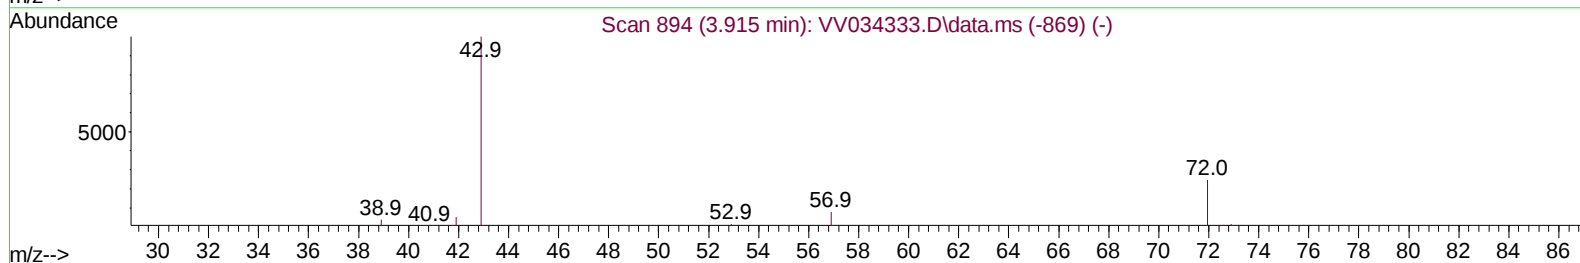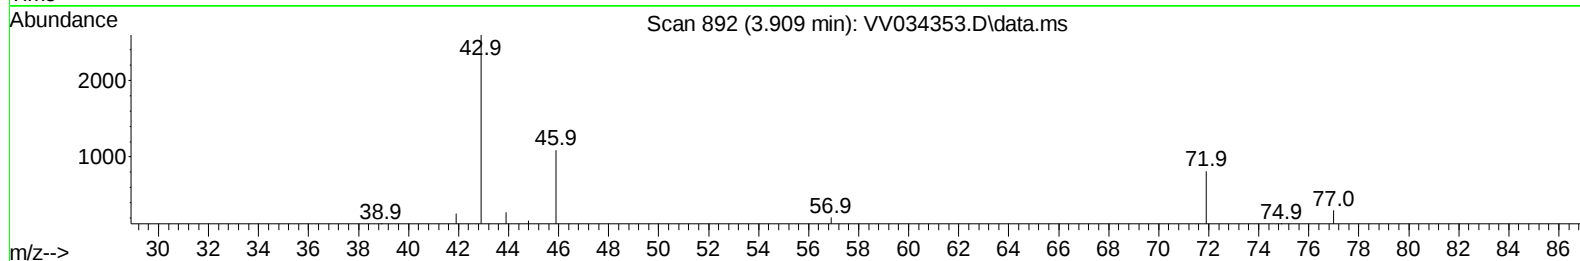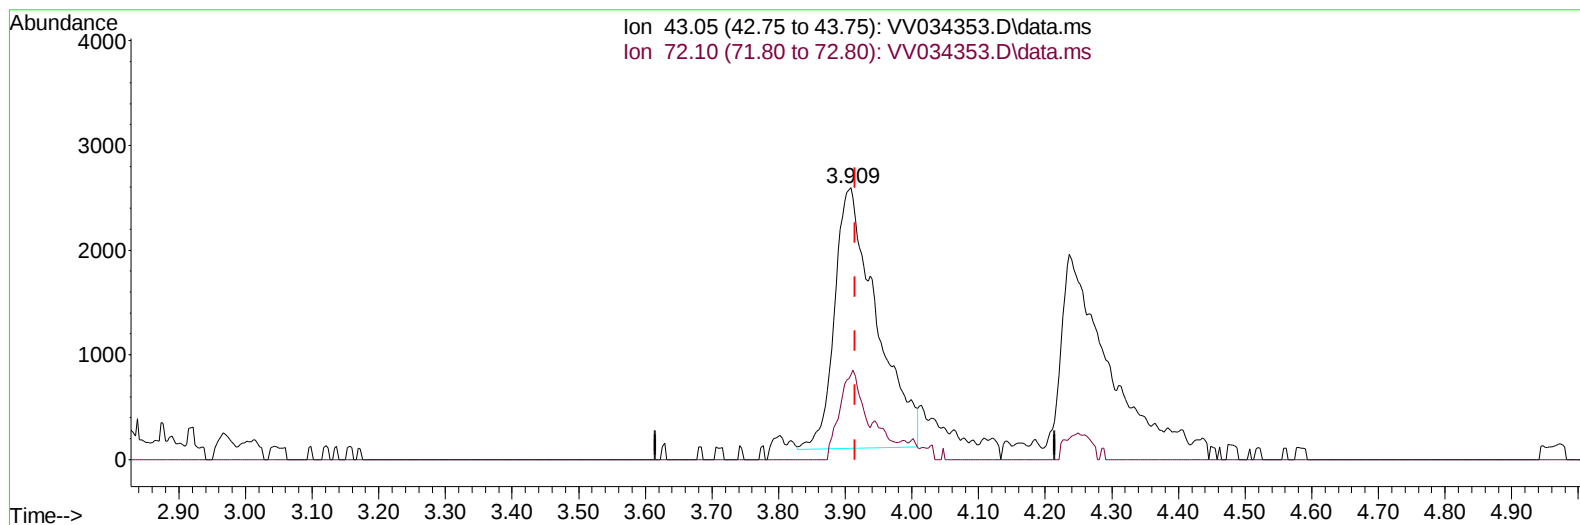

TIC: VV034353.D\data.ms

(21) 2-Butanone (T)

3.909min (-0.006) 11.28 ug/L

response 10871

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	7.90	18.74#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022224\
Data File : VV034353.D
Acq On : 22 Feb 2024 17:42
Operator : SY/MD
Sample : P1566-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAC0

Manual IntegrationsAPPROVED

Quant Time: Feb 23 01:19:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 23 01:14:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/23/2024
Supervised By :Semsettin Yesilyurt 02/23/2024

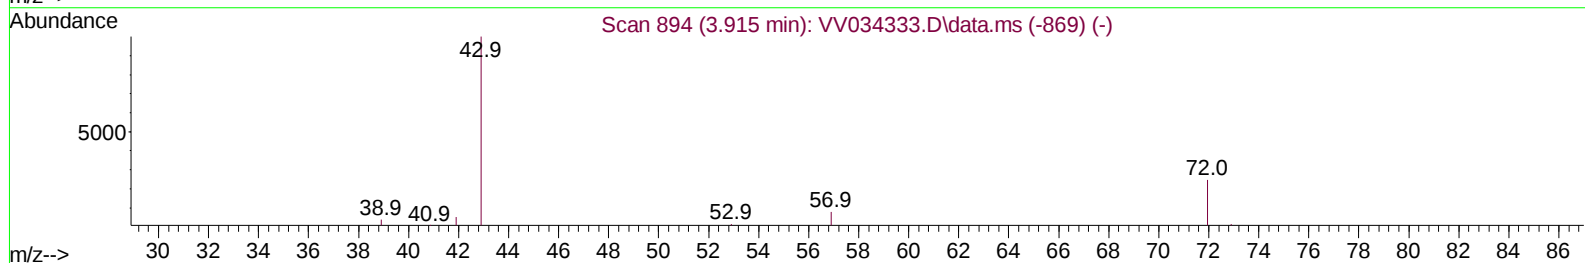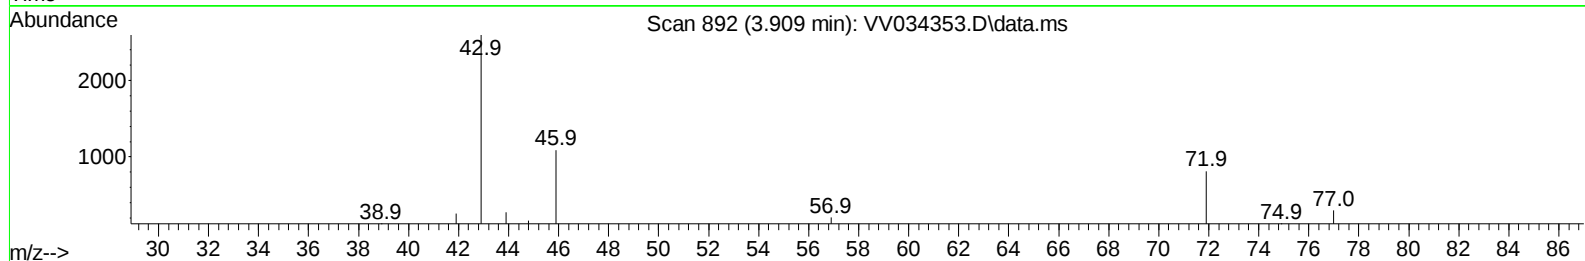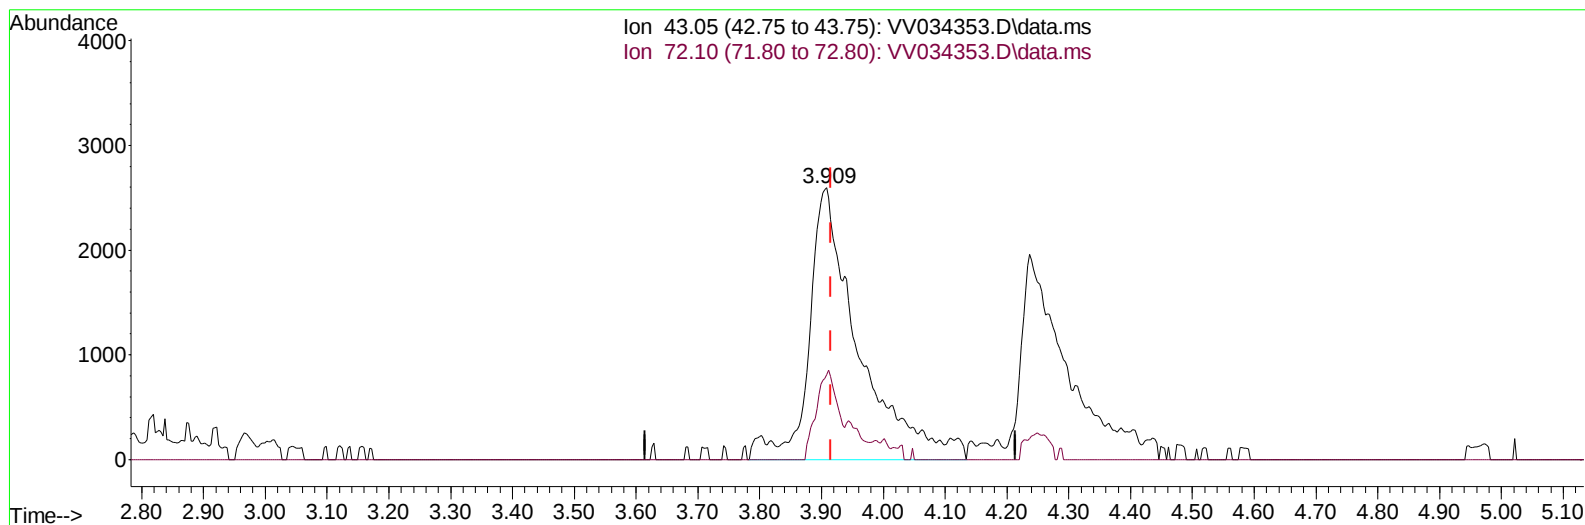

TIC: VV034353.D\data.ms

(21) 2-Butanone (T)

3.909min (-0.006) 14.97 ug/L m

response 14427

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	7.90	14.12#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022224\
 Data File : VV034353.D
 Acq On : 22 Feb 2024 17:42
 Operator : SY/MD
 Sample : P1566-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWACO

Manual IntegrationsAPPROVED

Quant Time: Feb 23 01:19:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 23 01:14:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/23/2024
 Supervised By :Semsettin Yesilyurt 02/23/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		73911	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		69389	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		33498	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		18027	3.149	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	63.000%	
7) Chloroethane-d5	1.532	69		18961	3.782	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	75.600%	
11) 1,1-Dichloroethene-d2	2.060	65		9790	3.546	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	71.000%	
20) 2-Butanone-d5	3.802	46		61162	63.620	ug/L	-0.03
Spiked Amount 50.000	Range 40	- 130		Recovery	=	127.240%	
24) Chloroform-d	4.249	84		51486	4.950	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	99.000%	
26) 1,2-Dichloroethane-d4	4.944	65		26204	5.391	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	107.800%	
32) Benzene-d6	4.963	84		91108	4.376	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	87.600%	
36) 1,2-Dichloropropane-d6	5.992	67		27871	4.789	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	95.800%	
41) Toluene-d8	7.243	98		80872	4.227	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	84.600%	
43) trans-1,3-Dichloroprop...	7.561	79		7982	3.632	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	72.600%	
46) 2-Hexanone-d5	8.027	63		46598	59.404	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	118.800%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84		20650	5.853	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	117.000%	
66) 1,2-Dichlorobenzene-d4	11.561	152		31049	5.097	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	102.000%	
Target Compounds							
13) Acetone	2.127	43		244562	335.319	ug/L #	37
21) 2-Butanone	3.909	43		14427m	14.969	ug/L	
47) Tetrachloroethene	7.908	164		4713	0.963	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022224\
Data File : VV034353.D
Acq On : 22 Feb 2024 17:42
Operator : SY/MD
Sample : P1566-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
JWAC0

Manual IntegrationsAPPROVED

Quant Time: Feb 23 01:19:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 23 01:14:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/23/2024
Supervised By :Semsettin Yesilyurt 02/23/2024

