




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022224\
Data File : VV034355.D
Acq On : 22 Feb 2024 18:31
Operator : SY/MD
Sample : P1566-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAC4

Manual IntegrationsAPPROVED

Quant Time: Feb 23 01:19:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 23 01:14:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/23/2024
Supervised By :Semsettin Yesilyurt 02/23/2024

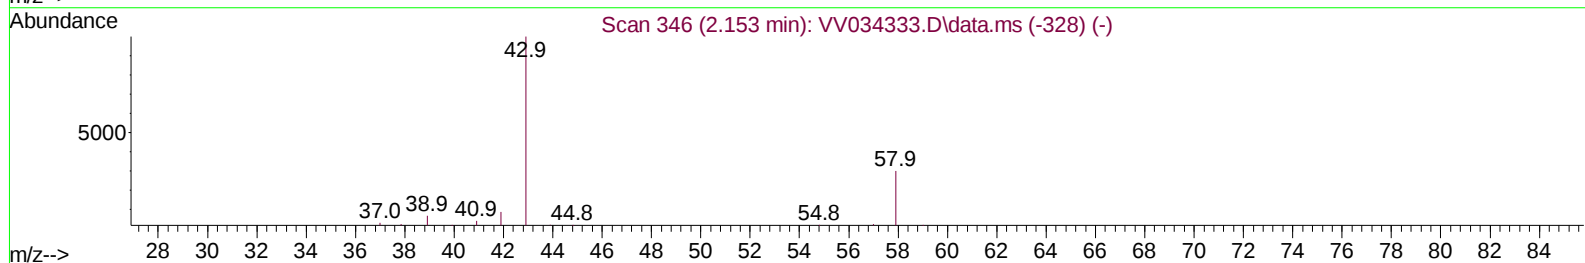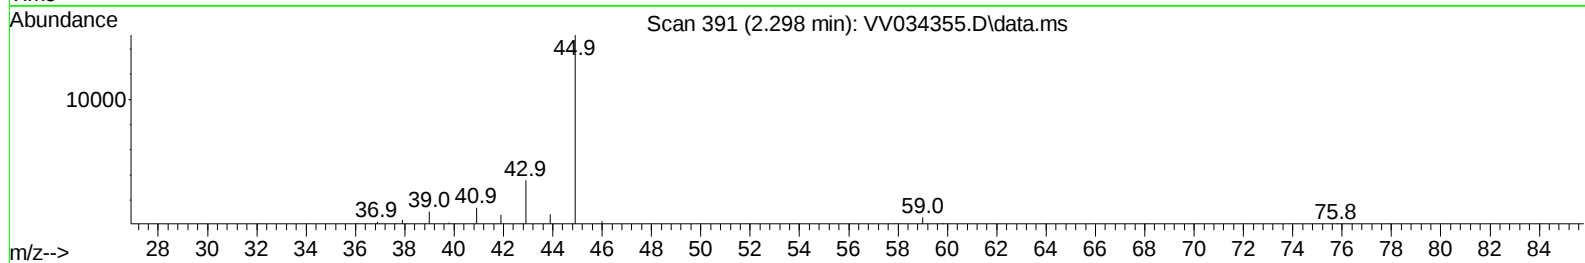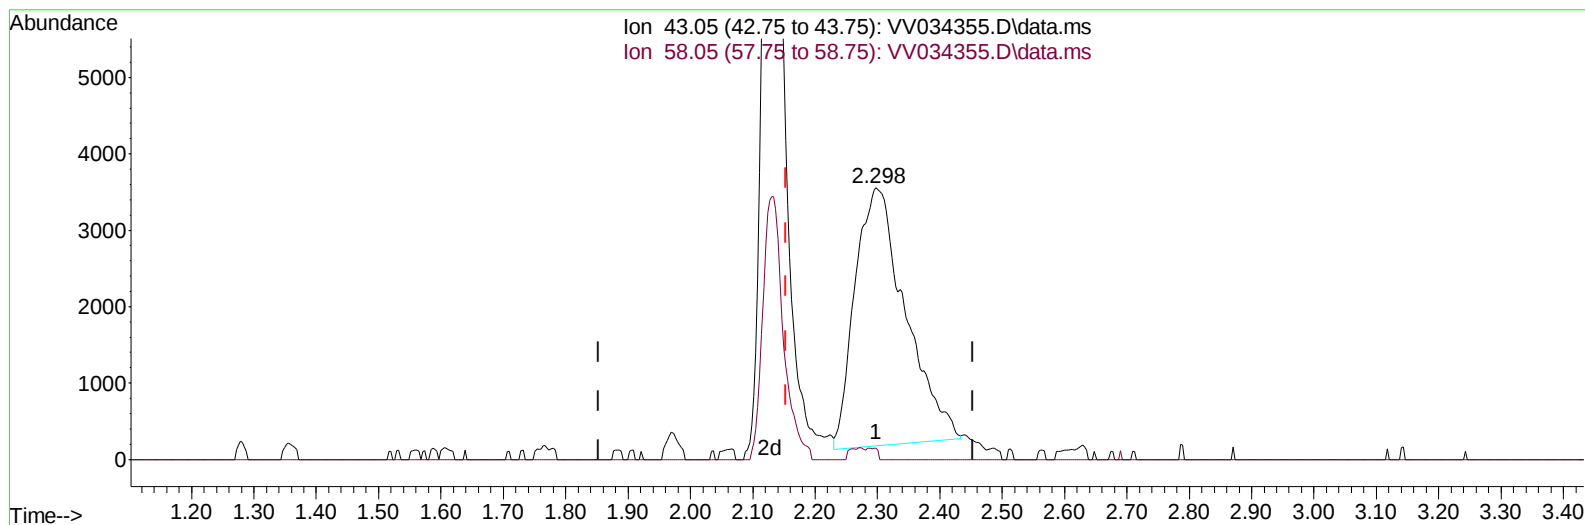

TIC: VV034355.D\data.ms

(13) Acetone (T)

2.298min (+ 0.145) 26.37 ug/L

response 18915

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	6.90	1.37
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022224\
 Data File : VV034355.D
 Acq On : 22 Feb 2024 18:31
 Operator : SY/MD
 Sample : P1566-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAC4

Manual IntegrationsAPPROVED

Quant Time: Feb 23 01:19:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 23 01:14:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/23/2024
 Supervised By :Semsettin Yesilyurt 02/23/2024

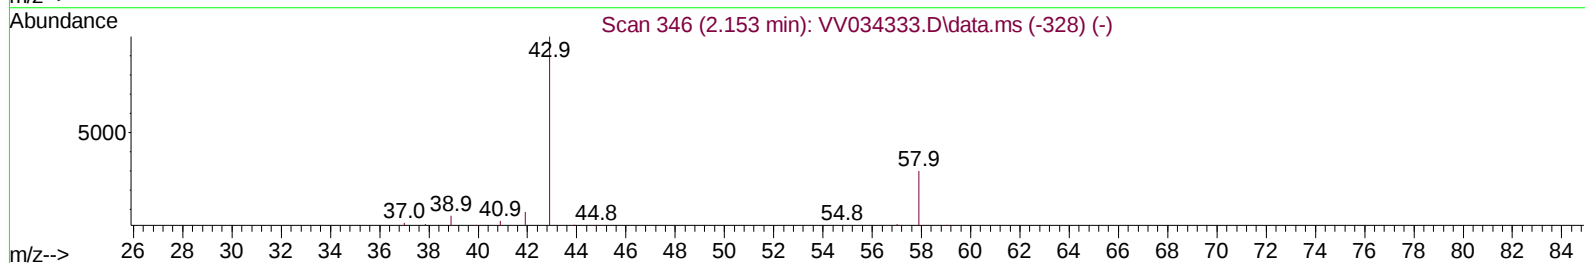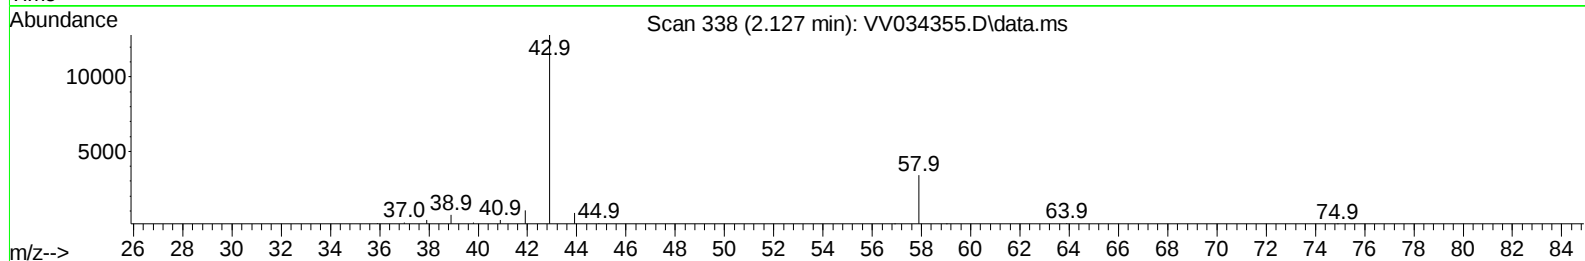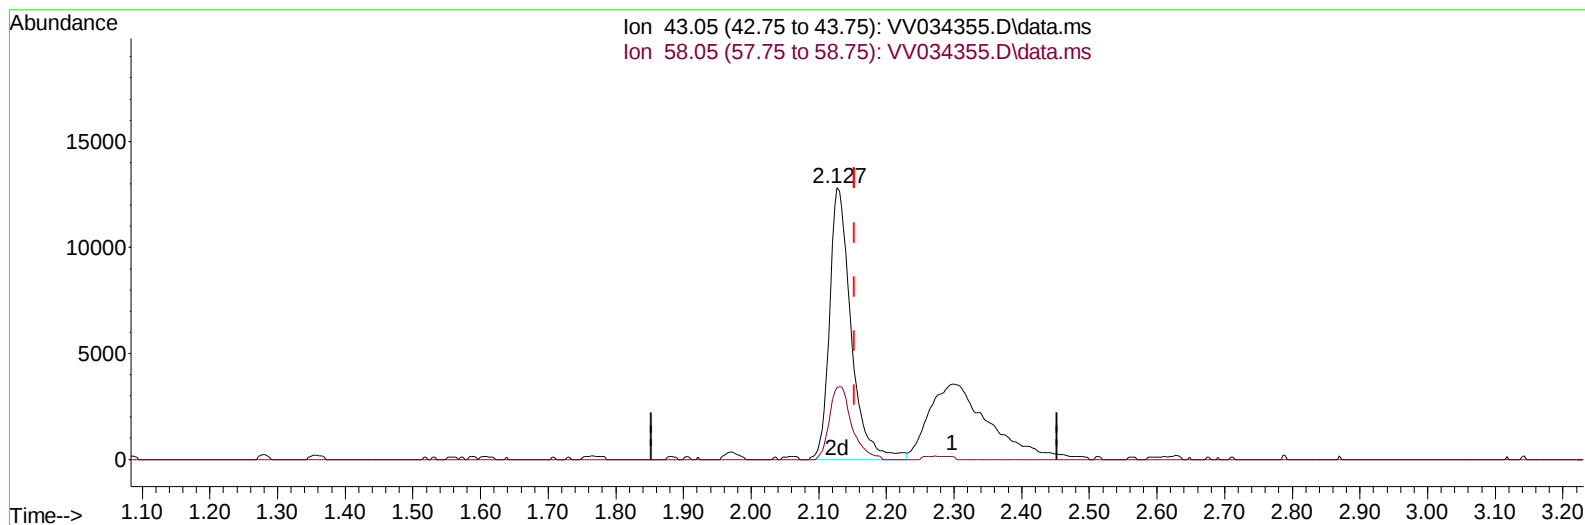

TIC: VV034355.D\data.ms

(13) Acetone (T)

2.127min (-0.026) 39.61 ug/L m

response 28410

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	6.90	0.92
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022224\
 Data File : VV034355.D
 Acq On : 22 Feb 2024 18:31
 Operator : SY/MD
 Sample : P1566-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAC4

Manual IntegrationsAPPROVED

Quant Time: Feb 23 01:19:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 23 01:14:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/23/2024
 Supervised By :Semsettin Yesilyurt 02/23/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		72678	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		67303	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		31886	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		17645	3.135	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	62.600%		
7) Chloroethane-d5	1.532	69		18387	3.729	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	74.600%		
11) 1,1-Dichloroethene-d2	2.060	65		9605	3.538	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	70.800%		
20) 2-Butanone-d5	3.802	46		58877	62.282	ug/L	-0.03
Spiked Amount 50.000	Range 40	- 130		Recovery =	124.560%		
24) Chloroform-d	4.252	84		49794	4.868	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	97.400%		
26) 1,2-Dichloroethane-d4	4.947	65		25436	5.322	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	106.400%		
32) Benzene-d6	4.963	84		87232	4.320	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	86.400%		
36) 1,2-Dichloropropane-d6	5.989	67		26598	4.712	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	94.200%		
41) Toluene-d8	7.246	98		79065	4.260	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	85.200%		
43) trans-1,3-Dichloroprop...	7.561	79		8513	3.994	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	79.800%		
46) 2-Hexanone-d5	8.027	63		44175	58.061	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	116.120%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84		20592	6.018	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	120.400%#		
66) 1,2-Dichlorobenzene-d4	11.561	152		31222	5.384	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	107.600%		
Target Compounds							
3) Chloromethane	1.217	50		2956	0.407	ug/L	92
13) Acetone	2.127	43		28410m	39.614	ug/L	
34) Trichloroethene	5.838	95		25425	4.352	ug/L	97
47) Tetrachloroethene	7.905	164		34322	7.230	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022224\
Data File : VV034355.D
Acq On : 22 Feb 2024 18:31
Operator : SY/MD
Sample : P1566-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAC4

Manual IntegrationsAPPROVED

Quant Time: Feb 23 01:19:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 23 01:14:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/23/2024
Supervised By :Semsettin Yesilyurt 02/23/2024

